

INCH-POUND

MIL-C-17G
AMENDMENT 3
8 JANUARY 1996
SUPERSEDING
AMENDMENT 2
9 JANUARY 1995

MILITARY SPECIFICATION

CABLES, RADIO FREQUENCY, FLEXIBLE AND SEMIRIGID, GENERAL SPECIFICATION FOR

This amendment forms a part of MIL-C-17G, dated 9 March 1990, and is approved for use by all Departments and Agencies of the Department of Defense.

PAGE 2

- * 2.1.1 Specifications, standards and handbooks; Delete reference to "TT-P-320" in its entirety.

PAGE 10

- * 3.5.7b, Delete this requirement. Existing stock (covered with aluminum paint) may be used until stock is purged.

PAGE 13

3.8, line 2: Delete "manufacturer's code symbol and name" and substitute "manufacturer's code symbol or name, and date code (date code to be marked on cable reel as a minimum)."

3.8b, item (2), add new sentence at end of entry: "If additional marking is possible, the remainder of the required military marking shall be applied."

PAGE 14

Delete section 4.1 Through 4.7.2.1.3 and substitute the following:

"4. QUALITY ASSURANCE PROVISIONS

"4.1 Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any other facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

"4.1.1 Responsibility for compliance. All items shall meet all requirements of sections 3 and 5. The inspection set forth in this specification shall become a part of the contractor's overall inspection system or quality program. The absence of any inspection requirements in the specification shall not relieve the contractor of the responsibility of ensuring that all products or supplies submitted to the Government for acceptance comply with all requirements of the contract. Sampling inspection, as part of manufacturing operations, is an acceptable practice to ascertain conformance to requirements, however this does not authorize submission of known defective material, either indicated or actual, nor does it commit the Government to accept defective material.

"4.1.2 Test equipment and inspection facilities. Test and measuring equipment and inspection facilities of sufficient accuracy, quality, and quantity to permit performance of the required inspection shall be established and maintained by the contractor. The establishment and maintenance of a calibration system to control the accuracy of the measuring and test equipment shall be in accordance with MIL-STD-45662.

MIL-C-17G
AMENDMENT 3

"4.1.3 Reliability assurance program. A reliability assurance program shall be established and maintained. Process control records shall cover the implementation of devices such as control charts (e.g., X bar and R charts) or other means of indication of the degree of control achieved in the production process. Records shall also indicate the action taken when each out-of-control condition is observed, and the disposition of non-conforming products processed during the period of out-of-control operation. Records associated with non-conforming products shall be kept for a minimum of 3 years. Evidence of such compliance shall be verified by the qualifying activity of this specification as a prerequisite for qualification and continued qualification."

"4.2 Classification of inspections. The inspections specified herein are classified as follows:

- a. Materials inspection (see 4.4).
- b. Final inspection (see 4.5).
- c. Qualification inspection (see 4.6).
- d. Quality conformance inspection (see 4.7).

"4.3 Inspection conditions. Unless otherwise specified herein, all test inspection conditions shall be performed in accordance with the test conditions specified in the General Requirements of MIL-STD-202, as follows:

- a. Temperature: 25°C ±10°C.
- b. Relative humidity: 60 percent ±15 percent.
- c. Atmospheric pressure: 725 mm ±75 mm of mercury.

"4.4 Materials inspection. Materials inspection shall consist of certification supported by verifying data that the materials listed in table II, used in fabricating the cables, are in accordance with the applicable referenced specifications or requirements prior to such fabrication."

MIL-C-17G
AMENDMENT 3

"TABLE II. Materials inspection.

Material	Requirement paragraph	Applicable documents
Ethylene tetrafluoroethylene (ETFE)	3.5.6k	ASTM D-3159
Ethylene chlorotrifluoroethylene (E-CTFE)	3.5.6l	ASTM D-3275
Fiberglass	3.5.6d	MIL-Y-1140
Fluorinated ethylene propylene (FEP)	3.5.2.1t	L-P-389
Paint, aluminum	3.5.7b	TT-P-320
Polyethylene (PE)	3.5.2.1a	L-P-390
Polytetrafluoroethylene (PTFE)	3.5.6f	ASTM D-1457
Polyolefin, cross-linked	3.5.6o	
Rubber, butyl, insulating synthetic	3.5.2.1s	ASTM D-1352
Rubber, insulating synthetic	3.5.2.1x	ASTM D-470
Rubber, polychloroprene	3.5.6a, c, e, i	MIL-I-3930
Rubber, synthetic, semiconductor	3.5.2.1r	FED-STD-601
Tape, polyethylene-terephthalate	3.5.5c	MIL-I-631
Tubing, aluminum, seamless	3.5.3.2b	WW-T-700
Tubing, copper, seamless	3.5.3.2a	WW-T-799
Wire, aluminum-alloy (alclad 5056)	3.5.7a	ASTM B-211
Wire, aluminum, copper-clad	3.5.1.1g	ASTM B-566
Wire, copper, bare	3.5.1.1a	ASTM B-3
Wire, copper, beryllium (alloy 172)	3.5.1.1h	ASTM B-197
Wire, copper, silver-coated	3.5.1.1c, j	ASTM B-298
Wire, copper, tin-coated	3.5.1.1b	ASTM B-33
Wire, high resistance	3.5.1.1k	QQ-R-175
Wire, steel, copper-clad	3.5.1.1d	ASTM B-452
Wire, steel, copper-clad, silver-coated	3.5.1.1f	ASTM B-501
Wire, steel, galvanized	3.5.3.1.1	ASTM A-411
Rubber, polyurethane	3.5.6m	MIL-I-3930
Stranded inner conductors	3.5.1.2	ASTM B-8
Copper conductors for use in hook-up wire for electronic equipment	3.5.1.2	ASTM B-286

"TABLE III. Final inspection.

Inspection		Requirement paragraph	Test method paragraph
Semirigid cable 1/	All other cable 2/		
Continuity	Continuity	3.7.1	4.8.2
Voltage withstanding	Spark test	3.7.2	4.8.3
	Voltage withstanding	3.7.3	4.8.4
	Insulation resistance	3.7.4	4.8.5
	Out-of-roundness of jacket measurements	3.6.2	4.8.1.2

1/ Sampling and inspection shall be in accordance with table VIII.

2/ Tests performed on each continuous length of cable."

"4.5 Final inspection. Prior to the delivery of the cable, the tests in table III shall be performed, as applicable.

"4.5.1 Failure.

- Semirigid cable - One or more failures shall be cause for refusal of lot.
- All other cable - One or more failures shall be cause for refusal of lot, except a spark test failure may be repaired or the cable length cut out.

"4.6 Qualification inspection. Qualification inspection shall be performed at a laboratory acceptable to the Government (see 6.3) on sample units produced with equipment and procedures normally used in production. Group qualification shall be as specified in the appendix to this specification.

"4.6.1 Sample. The sample of each cable type submitted for qualification inspection shall be of sufficient length to perform all the applicable tests in table IV.

MIL-C-17G
AMENDMENT 3

"4.6.2 Inspection routine. The samples shall be subjected to the inspections specified in table IV. The entire sample shall be subjected to the inspections of group I. The specimen length shall be cut from each sample as required, and subjected to inspections of group II.

"4.6.3 Failure. One or more failures shall be cause for refusal to grant qualification approval."

"TABLE IV. Qualification inspection.

Inspection	Number of specimens to be tested	Requirement paragraph	Test method paragraph
<u>Group I</u>			
In-process inspection	Entire sample		4.5
Continuity	Entire sample	3.7.1	4.8.2
Spark test	Entire sample	3.7.2	4.8.3
Voltage withstanding	Entire sample	3.7.3	4.8.4
Insulation resistance 1/	Entire sample	3.7.4	4.8.5
Visual and mechanical inspection	Entire sample	3.6	4.8.1
Physical dimensions	Entire sample	3.6	4.8.1
Marking	Entire sample	3.8	4.8.1
Workmanship	Entire sample	3.10	4.8.1
<u>Group II</u>			
Corona extinction voltage 2/	1	3.7.5	4.8.6
Characteristic impedance	1	3.7.6	4.8.7
RF transmission loss (attenuation) 2/	2	3.7.7	4.8.8
Standing wave ratio (return loss) 2/	2	3.7.8	4.8.9
Capacitance 2/	1	3.7.9	4.8.10
Capacitance stability 2/	1	3.7.10	4.8.11
Capacitance unbalance 3/	1	3.7.11	4.8.12
Transmission unbalance 3/	1	3.7.12	4.8.13
Mechanically induced noise voltage 4/	1	3.7.13	4.8.14
Time delay 2/	2	3.7.14	4.8.15
Aging stability 5/	4	3.7.15	4.8.16
Stress-crack resistance 2/	4	3.7.16	4.8.17
Outer conductor integrity 6/	4	3.7.17	4.8.18
Cold bend 2/	3	3.7.18	4.8.19
Dimensional stability 2/	1	3.7.19	4.8.20
Contamination 8/	1	3.7.20	4.8.21
Bendability 6/	2	3.7.21	4.8.22
Flammability 2/	1	3.7.22	4.8.23
Flame propagation 10/	1	3.7.23	4.8.24
Acid gas generation 10/	1	3.7.24	4.8.25
Halogen content 10/	1	3.7.25	4.8.26
Immersion 10/	1	3.7.26	4.8.27
Smoke index 10/	1	3.7.27	4.8.28
Toxicity index 10/	1	3.7.28	4.8.29
Durometer 10/	1	3.7.29	4.8.30
Weathering 10/	1	3.7.30	4.8.31
Abrasion resistance 10/	5	3.7.31	4.8.32
Tear strength 10/	6	3.7.32	4.8.33
Heat distortion 10/	1	3.7.33	4.8.34
Physicals (aged) 10/	1	3.7.34	4.8.35
Tensile strength and elongation 10/	1	3.7.35	4.8.36
Weight	1	3.9	4.8.37

1/ Not applicable to solid types A and F dielectric cores.

2/ When specified.

3/ Applicable to two-conductor cables.

4/ Applicable to low noise cables.

5/ Not applicable to semirigid or cables with type IX jackets.

6/ Applicable to semirigid cables.

MIL-C-17G
AMENDMENT 3

7/ Not applicable to time delay or braided inner conductor cables.

8/ Applicable to type IIA jackets.

9/ Not applicable to semirigid cables.

10/ Applicable to type XIV, polyolefin jacketed cables only."

"4.6.4 Retention of qualification. To retain qualification, the contractor shall forward a report at 12-month intervals to the qualifying activity. The qualifying activity shall establish the initial reporting date. The report shall consist of:

- a. A summary of the results of the tests performed for inspection of product for delivery (groups A and B), indicating as a minimum the number of lots that have passed and the number that have failed.
- b. A summary of the results of tests performed for qualification verification inspection group C, including the number and mode of failures. The summary shall include results of all qualification verification inspection tests performed and completed during the 12-month period. If the summary of the test results indicates nonconformance with specification requirements, and corrective action acceptable to the qualifying activity has not been taken, action may be taken to remove the failing product from the qualified products list.

Failure to submit the report within 30 days after the end of each 12-month period may result in loss of qualification for the product. In addition to the periodic submission of inspection data, the contractor shall immediately notify the qualifying activity at any time during the 12-month period that the inspection data indicates failure of the qualified product to meet the requirements of this specification.

In the event that no production occurred during the reporting period, a report shall be submitted certifying that the company still has the capabilities and facilities necessary to produce the item. If during three consecutive reporting periods there has been no production, the manufacturer may be required, at the discretion of the qualifying activity, to submit representative cables of each type to testing in accordance with the qualification inspection requirements.

"4.7 Quality conformance inspection.

"4.7.1 Inspection of product for delivery. Inspection and final inspection in accordance with table III of product for delivery shall consist of groups A and B inspections.

"4.7.1.1 Unit of product. A unit of product shall be 5,000 feet of cable of the same type designation. If a production run is less than 5,000 feet, then the quantity produced shall be one unit of product.

"4.7.1.1.1 Inspection lot. The inspection lot shall consist of the number of units of product, offered for inspection at one time. All of the units of product in the inspection lot submitted shall have been produced during the same production period with the same materials and processes.

"4.7.1.1.2 Sample unit. A sample unit shall be a unit of product selected at random from the inspection lot without regard to quality.

"4.7.1.1.3 Sample unit size. Unless otherwise specified, the sample unit size shall consist of that number of sample units required by the inspection lot size, as determined by table VIII.

"4.7.1.1.4 Specimen. A specimen shall be an individual length of cable cut from the sample unit.

"4.7.1.2 Group A inspection. Group A inspection shall consist of the inspections specified in table V.

"4.7.1.2.1 Sampling plan. Table V, tests shall be performed on a production lot basis. Samples shall be selected in accordance with table VIII. If one or more defects are found, the lot shall be screened for that particular defect(s) and defects removed. A new sample of product shall be selected in accordance with table VIII and all group A tests for previously found defects shall again be performed. If any defects are found in the second sample, the lot shall be rejected and shall not be supplied to this specification.

"4.7.1.2.1.1 Visual inspection (group A). Each cable shall be visually examined for completeness, workmanship and identification requirements."

MIL-C-17G
AMENDMENT 3

"TABLE V. Group A inspection.

Inspection	Requirement paragraph	Test method paragraph
Visual and mechanical inspection	3.6	4.8.1
Physical dimensions	3.6	4.8.1
Marking	3.8	4.8.1
Workmanship	3.10	4.8.1
Characteristic impedance	3.7.6	4.8.7
RF transmission loss (attenuation)	3.7.7	4.8.8
Standing wave ratio (return loss)	3.7.8	4.8.9
1/	3.6.4	4.8.1.4
Adhesion of conductors	3.6.3	4.8.1.3
Eccentricity of inner conductor		

1/ As applicable."

"4.7.1.3 Group B inspection. Group B inspection shall consist of the inspections specified in table VI.

"4.7.1.3.1 Sampling plan. The sampling plan shall be in accordance with table VIII. If one or more defects are found, the lot shall be screened for that particular defect(s) and defects removed. A new sample of product shall be selected in accordance with table VIII and all group B tests for previously found defects shall again performed. If any defects are found in the second sample, the lot shall be rejected and shall not be supplied to this specification."

"TABLE VI. Group B inspection.

Inspection	Requirement paragraph	Test method paragraph
Corona extinction voltage 1/	3.7.5	4.8.6
Capacitance	3.7.9	4.8.10
Capacitance unbalance 1/	3.7.11	4.8.12
Transmission unbalance 1/	3.7.12	4.8.13
Mechanically induced noise voltage	3.7.13	4.8.14
1/	3.7.14	4.8.15
Time delay 1/	3.7.18	4.8.19
Cold bend 2/	3.9	4.8.24
Weight	3.7.32	4.8.34
Tear strength		

1/ As applicable.

2/ Not applicable to semirigid cables."

"4.7.2 Group C inspection. Group C inspection shall consist of the inspections specified in table VII. group C inspection shall be made on sample units selected from inspection lots which have passed the groups A and B inspection.

"4.7.2.1 Sampling plan. Sample units shall be selected from those types covered by a single specification sheet in accordance with table VIII, 3 months after the date of notification of qualification, except when the total production in a 3-month period is less than two units of product (10,000 feet) inspection need not be made until either production is at least 2 units of product or a total of 6 months has elapsed since the inspection was performed in which case only one sample unit shall be tested."

MIL-C-17G
AMENDMENT 3

"TABLE VII. Group C inspection.

Inspection	Requirement paragraph	Test method paragraph
Capacitance stability	3.7.10	4.8.11
Aging stability 1/	3.7.15	4.8.16
Stress-crack resistance	3.7.16	4.8.17
Outer conductor integrity	3.7.17	4.8.18
Dimensional stability	3.7.19	4.8.20
Contamination 2/	3.7.20	4.8.21
Bendability 1/	3.7.21	4.8.22
Flammability 1/	3.7.22	4.8.23
Heat distortion 1/	3.7.33	4.8.35
Tensile strength and elongation	3.7.35	4.8.37
1/	3.7.34	4.8.36
Physicals (aged) 1/		

1/ When specified.

2/ Applicable to type IIa jackets."

"TABLE VIII. Sampling plan for all group inspection.

Units of product from 3-month's production	Sample unit size
2	1
3 to 8 inclusive	2
9 to 30 inclusive	3
31 to 80 inclusive	4
81 to 130 inclusive	5
131 to 180 inclusive	6
181 to 240 inclusive	7
241 to 300 inclusive	8

"4.7.2.1.1 Failures. If one or more specimens fail to pass group C inspection, the inspection lot shall be considered to have failed.


"4.7.2.1.2 Disposition of specimens. Specimens that have been tested to group C inspection shall not be delivered on the contract or purchase order.

"4.7.2.1.3 Noncompliance. If a sample fails to pass group C inspection, the manufacturer shall notify the qualifying activity and the cognizant inspection activity of such failure and take corrective action on the materials or processes, or both, as warranted, and on all units of product which can be corrected and which are manufactured under essentially the same materials and processes, and which are considered subject to the same failure. Acceptance and shipment of the product shall be discontinued until corrective action, acceptable to the qualifying activity has been taken. After the corrective action has been taken group C inspection shall be repeated on additional sample units (all tests and examinations, or the test which the original sample failed, at the option of the qualifying activity). Groups A and B inspections may be reinstituted; however, final acceptance and shipment shall be withheld until the group C inspection has shown that the corrective action was successful. In the event of failure after reinspection, information concerning the failure shall be furnished to the cognizant inspection activity and the qualifying activity."

MIL-C-17G
AMENDMENT 3

PAGE 34

FIGURE 8, delete and substitute new figure 8 as printed below:

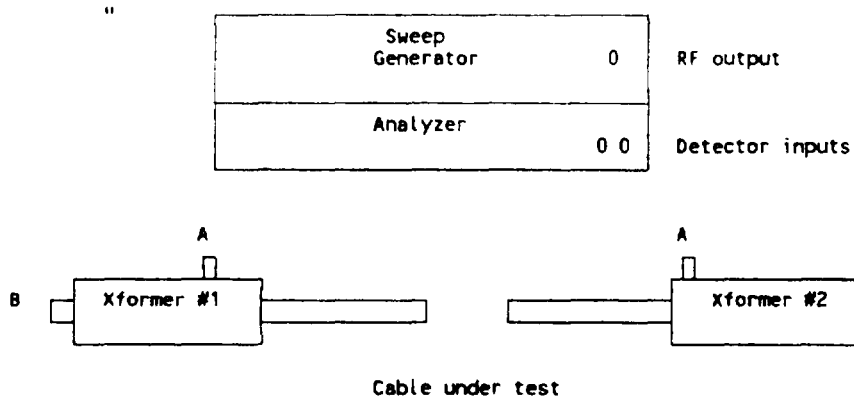

Port A and B are series N connectors, remaining two are twinaxial.

FIGURE 8. Transmission unbalance."

PAGE 35

4.8.13.4, delete and substitute the following:

***4.8.13.4 Transmission unbalance test procedure.** The following test procedure or one suitable to the Government shall be used for measuring transmission unbalance. In the event of conflict, the following method shall be the referee test.

Equipment used: Sweep generator (set to sweep 100-160 MHz).
Analyzer and printer.
1 or 2 RF detectors.
2 Telplex (Alford) transformers w/calibration device.
1 or 2 50-ohm loads.

Procedure:

1. Detectors shall be calibrated to obtain a zero reference line.
2. Connect the RF output of the generator to port A or B of transformer #1.
3. To the other port place a 50-ohm load.
4. Connect the calibration device between the two transformers.
5. To transformer #2, connect the RF detector from port A of the analyzer to port A of the transformer and a 50-ohm load to port B.
6. If a second RF detector is available, then connect it from port B of the analyzer to port B of the transformer.
7. Obtain a trace on the analyzer from port A. If two detectors are used, then obtain two traces on the analyzer.
8. Calculate the minimum difference between the two traces in dB and using the following formula determine the unbalance. This number should be approximately 50-51 dB which equals less the 1% unbalance.

MIL-C-17G
AMENDMENT 3

$$TUB \% = \frac{200}{\left(\text{antilog}_{10} \frac{\text{dB difference}}{20} \right)}$$

9. Change the detector from port A of the transformer to port B, and the load to port A.
10. When these are printed, the resulting unbalance shall be calculated as in step 7 above.
11. Remove the calibration device and place the cable to be tested between the two ports of the transformer.
12. Repeat steps 5-10, as appropriate.
13. See table X for the minimum unbalance allowable."

PAGE 47

4.8.32, Irradiance entry: Delete ".nm". Also for Arc lamp off entry: Delete "35 ±2°C" and substitute "25°C ±2°C".

The margins of this amendment are marked with an asterisk to indicate where changes (additions, modifications, corrections, deletions) from the previous amendment were made. This was done as a convenience only, and the Government assumes no liability whatsoever for any inaccuracies in these notations. Bidders and contractors are cautioned to evaluate the requirements of this document based on the entire content irrespective of the marginal notations and relationship to the last previous amendment.

CONCLUDING MATERIAL

Custodians:

Army - CR
Navy - EC
Air Force - 85

Preparing activity:
DLA-ES

(Project 6145-2119)

Review activities:

Army - AR, AT, ME, MI
Navy - AS, MC, OS, SH
Air Force - 17, 19, 99
NASA - NA
DLA - IS

MILITARY SPECIFICATION

CABLES, RADIO FREQUENCY, FLEXIBLE AND SEMIRIGID,
GENERAL SPECIFICATION FOR

This amendment forms a part of MIL-C-17G, dated 9 March 1990, and is approved for use by all Departments and Agencies of the Department of Defense.


PAGE 13

3.8, line 2: Delete "manufacturer's code symbol and name" and substitute "manufacturer's code symbol or name, and date code".

3.8b, item (2), add new sentence at end of entry: "If additional marking is possible, the remainder of the required military marking shall be applied."

PAGE 34

FIGURE 8, delete and substitute new figure 8 as printed below:

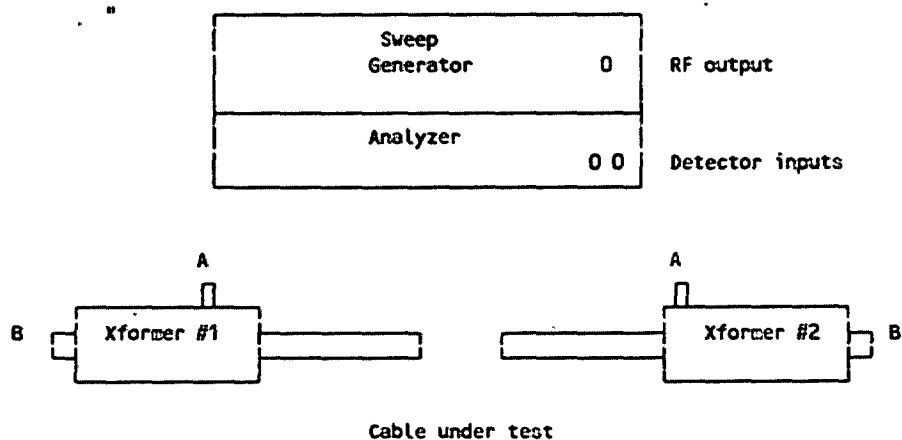

Port A and B are series N connectors, remaining two are twinaxial.

FIGURE 8. Transmission unbalance."

4.8.13.4, delete and substitute the following:

"4.8.13.4 Transmission unbalance test procedure. The following test procedure or one suitable to the Government shall be used for measuring transmission unbalance. In the event of conflict, the following method shall be the referee test.

Equipment used: Sweep generator (set to sweep 100-160 MHz).
Analyzer and printer.
1 or 2 RF detectors.
2 Telplex (Alford) transformers w/calibration device.
1 or 2 50-ohm loads.

Procedure:

1. Detectors shall be calibrated to obtain a zero reference line.
2. Connect the RF output of the generator to port A or B of transformer #1.
3. To the other port place a 50-ohm load.
4. Connect the calibration device between the two transformers.
5. To transformer #2, connect the RF detector from port A of the analyzer to port A of the transformer and a 50-ohm load to port B.
6. If a second RF detector is available, then connect it from port B of the analyzer to port B of the transformer.
7. Obtain a trace on the analyzer from port A. If two detectors are used, then obtain two traces on the analyzer.
8. Calculate the minimum difference between the two traces in dB and using the following formula determine the unbalance. This number should be approximately 50-51 dB which equals less the 1% unbalance.

$$TUB \% = \frac{200}{(\text{antilog}_{10} \frac{dB \text{ difference}}{20})}$$

9. Change the detector from port A of the transformer to port B, and the load to port A.
10. When these are printed, the resulting unbalance shall be calculated as in step 7 above.
11. Remove the calibration device and place the cable to be tested between the two ports of the transformer.
12. Repeat steps 5-10, as appropriate.
13. See table X for the minimum unbalance allowable."

4.8.32, Irradiance entry: Delete ".nm". Also for Arc lamp off entry: Delete "35 ±2°C" and substitute "25°C ±2°C".

CONCLUDING MATERIAL

Custodians:

Army - CR
Navy - EC
Air Force - 85

Preparing activity:
DLA-ES

Review activities:

Army - AR, AT, ME, MI
Navy - AS, MC, OS, SH
Air Force - 17, 19, 99
NASA - NA
DLA - IS

(Project 6145-2026)

INCH-POUND

MIL-C-17G
SUPPLEMENT 1
9 March 1990

MILITARY SPECIFICATION

CABLES, RADIO FREQUENCY, FLEXIBLE AND SEMIRIGID, GENERAL SPECIFICATION FOR

This supplement forms a part of Military Specification
MIL-C-17G, dated 9 March 1990

SPECIFICATION SHEETS

- MIL-C-17/2 - Cable, Radio Frequency, Flexible, Coaxial, 75 Ohms, M17/2-RG6.
- MIL-C-17/6 - Cables, Radio Frequency, Flexible, Coaxial, 75 Ohms, M17/6-RG11, Unarmored, M17/6-RG12, Armored.
- MIL-C-17/15 - Cables, Radio Frequency, Flexible, Twin, 95 Ohms, Unarmored M17/015-RG022, and Armored M17/015-RG111.
- MIL-C-17/16 - Cables, Radio Frequency, Flexible, Coaxial, Dual, 125 Ohms, M17/16-RG23 (Unarmored), M17/16-RG24 (Armored).
- MIL-C-17/19 - Cables, Radio Frequency, Flexible, Triaxial, Pulse, 48 Ohms, M17/19-RG25.
- MIL-C-17/21 - Cables, Radio Frequency, Flexible, Coaxial, Pulse, 48 Ohms, M17/21-RG26.
- MIL-C-17/22 - Cables, Radio Frequency, Flexible, Coaxial, Pulse, 48 Ohms, M17/22-RG27 (Armored), M17/22-00001 (Unarmored).
- MIL-C-17/23 - Cables, Radio Frequency, Flexible, Triaxial, Pulse, 48 Ohms, M17/23-RG28.
- MIL-C-17/24 - Cable, Radio Frequency, Flexible, Coaxial, 75 Ohms, M17/24-RG34.
- MIL-C-17/28 - Cables, Radio Frequency, Flexible, Coaxial, 50 Ohms, M17/028-RG058.
- MIL-C-17/29 - Cables, Radio Frequency, Flexible, Coaxial, 75 Ohms, M17/29-RG59.
- MIL-C-17/30 - Cables, Radio Frequency, Flexible, Coaxial, 93 Ohms, M17/030-RG062.
- MIL-C-17/31 - Cables, Radio Frequency, Flexible, Coaxial, 125 Ohms, M17/31-RG63, Unarmored, M17/31-RG79, Armored.
- MIL-C-17/33 - Cables, Radio Frequency, Flexible, Coaxial, Pulse, 48 Ohms, M17/33-RG64.
- MIL-C-17/34 - Cables, Radio Frequency, Flexible, Coaxial, Time Delay, 950 Ohms, M17/34-RG65.
- * MIL-C-17/40 - Cable, Radio Frequency, Coaxial, RG-85A/U.
- * MIL-C-17/43 - Cable, Radio Frequency, Coaxial, RG-88/U.
- MIL-C-17/45 - Cables, Radio Frequency, Flexible, Twin, 78 Ohms, M17/045-RG108.
- MIL-C-17/47 - Cable, Radio Frequency, Flexible, Coaxial, 185 Ohms, M17/47-RG114.
- MIL-C-17/52 - Cables, Radio Frequency, Flexible, Coaxial, 50 Ohms, M17/52-RG119, Unarmored, M17/52-RG120, Armored.
- MIL-C-17/54 - Cables, Radio Frequency, Flexible, Coaxial, 50 Ohms, M17/54-RG122.
- MIL-C-17/56 - Cables, Radio Frequency, Flexible, Twin, 95 Ohms, M17/56-RG130 (Unarmored), M17/56-RG131 (Armored).
- MIL-C-17/60 - Cables, Radio Frequency, Flexible, Coaxial, 50 Ohms, M17/60-RG142.
- MIL-C-17/62 - Cables, Radio Frequency, Flexible, Coaxial, 75 Ohms, M17/62-RG144.

* Inactive for new design.

MIL-C-17G
SUPPLEMENT 1

MIL-C-17/64 - Cables, Radio Frequency, Flexible, Coaxial, 75 Ohms, M17/64-RG164, Unarmored, M17/64-RG035, Armored.

MIL-C-17/65 - Cables, Radio Frequency, Flexible, Coaxial, 50 Ohms Unarmored M17/65-RG165, and Armored, M17/65-RG166.

MIL-C-17/67 - Cables, Radio Frequency, Flexible, Coaxial, 50 Ohms, M17/67-RG177.

MIL-C-17/72 - Cables, Radio Frequency, Flexible, Coaxial, 50 Ohms, M17/72-RG211.

MIL-C-17/73 - Cables, Radio Frequency, Flexible, Coaxial, 50 Ohms, M17/73-RG212.

MIL-C-17/74 - Cables, Radio Frequency, Flexible, Coaxial 50 Ohms, Unarmored M17/74-RG213, and Armored M17/74-RG215.

MIL-C-17/75 - Cables, Radio Frequency, Flexible, Coaxial, 50 Ohms, M17/75-RG214 and M17/75-RG365.

MIL-C-17/77 - Cable, Radio Frequency, Flexible, Coaxial, 75 Ohms M17/77-RG216.

MIL-C-17/78 - Cables, Radio Frequency, Flexible, Coaxial, 50 Ohms, M17/78-RG217.

MIL-C-17/79 - Cables, Radio Frequency, Flexible, Coaxial, 50 Ohms Unarmored M17/79-RG218, and Armored, M17/79-RG219.

* MIL-C-17/81 - Cable, Radio Frequency, Flexible, Coaxial, 50 ohms, M17/81-00001 and M17/81-00002 Armored.

MIL-C-17/84 - Cables, Radio Frequency, Flexible, Coaxial, 50 Ohms, M17/84-RG223.

MIL-C-17/86 - Cable, Radio Frequency, Coaxial, RG-225/U.

MIL-C-17/87 - Cable, Radio Frequency, Coaxial, RG-226/U.

MIL-C-17/90 - Cables, Radio Frequency, Coaxial, 93 Ohms, M17/90-RG71.

MIL-C-17/92 - Cable, Radio Frequency, Flexible, Coaxial, 50 Ohms, M17/92-RG115.

MIL-C-17/93 - Cable, Radio Frequency, Flexible, Coaxial, 50 Ohms, M17/93-RG178 and M17/93-00001.

MIL-C-17/94 - Cables, Radio Frequency, Flexible, Coaxial, 75 Ohms, M17/094-RG179.

MIL-C-17/95 - Cables, Radio Frequency, Flexible, Coaxial, 95 Ohms, M17/095-RG180.

MIL-C-17/97 - Cables, Radio Frequency, Flexible, Coaxial, 93 Ohms, M17/97-RG210.

MIL-C-17/100 - Cable, Radio Frequency, Flexible, Coaxial, 95 Ohms, M17/100-RG133.

MIL-C-17/110 - Cable, Radio Frequency, Flexible, Coaxial, 75 Ohms, M17/110-RG302.

MIL-C-17/111 - Cables, Radio Frequency, Flexible, Coaxial, 50 Ohms, M17/111-RG303.

MIL-C-17/112 - Cable, Radio Frequency, Flexible, Coaxial, M17/112-RG304.

MIL-C-17/113 - Cable, Radio Frequency, Flexible, Coaxial, 50 Ohms, M17/113-RG316.

MIL-C-17/116 - Cables, Radio Frequency, Flexible, Triaxial, 75 Ohms, M17/116-RG307.

MIL-C-17/119 - Cables, Radio Frequency, Flexible, Coaxial, 50 Ohms, M17/119-RG174.

MIL-C-17/124 - Cables, Radio Frequency, Flexible, Triaxial, Pulse, 25 Ohms, M17/124-RG328.

MIL-C-17/126 - Cables, Radio Frequency, Coaxial, Low Noise, 72 Ohms, M17/126-RG391 (Unarmored), M17/126-RG392 (Armored).

MIL-C-17/127 - Cable, Radio Frequency, Flexible, Coaxial, 50 Ohms, M17/127-RG393.

MIL-C-17/128 - Cable, Radio Frequency, Flexible, Coaxial, 50 Ohms, M17/128-RG400.

MIL-C-17/129 - Cables, Radio Frequency, Coaxial, 0.250 Diameter, Semirigid, 50 Ohms, M17/129-RG401 and M17/129-00001.

MIL-C-17/130 - Cables, Radio Frequency, Coaxial, 0.141 Diameter, Semirigid, 50 Ohms, M17/130-RG402 and M17/130-00001 through M17/130-00003.

MIL-C-17/131 - Cables, Radio Frequency, Flexible, Triaxial, 50 Ohms, M17/131-RG403.

MIL-C-17/132 - Cables, Radio Frequency, Coaxial, Low Noise, 50 Ohms, M17/132-RG404.

MIL-C-17/133 - Cables, Radio Frequency, Coaxial, 0.086 Diameter, Semirigid, 50 Ohms, M17/133-RG405, M17/133-00001 through -00005.

MIL-C-17/134 - Cable, Radio Frequency, Triaxial, 0.245 Inch, 50 Ohm Waterblocked, Non-Water Blocked.

MIL-C-17/135 - Cable, Radio Frequency, Triaxial, Diameter 0.500 Inch, 50 Ohm, Waterblocked and Non-Waterblocked.

MIL-C-17/136 - Cable, Radio Frequency, Flexible, Coaxial, 75 Ohms, M17/136-00001.

MIL-C-17/137 - Cable, Radio Frequency, Flexible, Coaxial, 95 Ohms, M17/137-00001.

MIL-C-17/138 - Cable, Radio Frequency, Flexible, Coaxial, 50 Ohms, M17/138-00001.

MIL-C-17/139 - Cable, Radio Frequency, Flexible, Coaxial, 95 Ohms, M17/139-00001.

MIL-C-17/151 - Cables, Radio Frequency, Coaxial, 0.047 Inch Diameter, Semirigid, 50 Ohms, M17/151-00001 and M17/151-00002.

* Inactive for new design.

**MIL-C-17G
SUPPLEMENT 1**

MIL-C-17/152 -	Cable, Radio Frequency, Flexible, Coaxial, 50 Ohms, M17/152-00001.
MIL-C-17/154 -	Cables, Radio Frequency, Coaxial, 0.034 Inch Diameter, Semirigid, 50 Ohms, M17/154-00001 and M17/154-00002.
MIL-C-17/155 -	Cables, Radio Frequency, Flexible, Coaxial, 50 Ohms, M17/155-00001.
MIL-C-17/156 -	Cables, Radio Frequency, Flexible, Coaxial, 50 Ohms, M17/156-00001.
MIL-C-17/157 -	Cables, Radio Frequency, Flexible, Coaxial, 50 Ohms, M17/157-00001.
MIL-C-17/158 -	Cables, Radio Frequency, Flexible, Coaxial, 50 Ohms, M17/158-00001.
MIL-C-17/159 -	Cables, Radio Frequency, Flexible, Coaxial, 50 Ohms, M17/159-00001.
MIL-C-17/160 -	Cables, Radio Frequency, Flexible, Coaxial, 50 Ohms, M17/160-00001.
MIL-C-17/161 -	Cables, Radio Frequency, Flexible, Coaxial, 50 Ohms, M17/161-00001.
MIL-C-17/162 -	Cables, Radio Frequency, Flexible, Coaxial, 50 Ohms, M17/162-00001.
MIL-C-17/163 -	Cables, Radio Frequency, Flexible, Coaxial, 50 Ohms, M17/163-00001.
MIL-C-17/164 -	Cables, Radio Frequency, Flexible, Coaxial, 50 Ohms, M17/164-00001.
MIL-C-17/165 -	Cables, Radio Frequency, Flexible, Coaxial, 50 Ohms, M17/165-00001.
MIL-C-17/166 -	Cables, Radio Frequency, Flexible, Coaxial, 50 Ohms, M17/166-00001.
MIL-C-17/167 -	Cables, Radio Frequency, Flexible, Coaxial, 50 Ohms, M17/167-00001.
MIL-C-17/168 -	Cables, Radio Frequency, Flexible, Coaxial, 50 Ohms, M17/168-00001.
MIL-C-17/169 -	Cables, Radio Frequency, Flexible, Coaxial, 50 Ohms, M17/169-00001.
MIL-C-17/170 -	Cables, Radio Frequency, Flexible, Coaxial, 50 Ohms, M17/170-00001.
MIL-C-17/171 -	Cables, Radio Frequency, Flexible, Coaxial, 50 Ohms, M17/171-00001.
MIL-C-17/172 -	Cables, Radio Frequency, Flexible, Coaxial, 50 Ohms, M17/172-00001.
MIL-C-17/173 -	Cables, Radio Frequency, Flexible, Coaxial, 50 Ohms, M17/173-00001.
MIL-C-17/174 -	Cables, Radio Frequency, Flexible, Coaxial, 50 Ohms, M17/174-00001.
MIL-C-17/175 -	Cables, Radio Frequency, Flexible, Coaxial, 50 Ohms, M17/175-00001.
MIL-C-17/176 -	Cables, Radio Frequency, Flexible, Twin, MIL-C-17/176-00002.
MIL-C-17/177 -	Cables, Radio Frequency, Flexible, Triaxial, 95 ohms, M17/177-00001.
MIL-C-17/178 -	Cables, Radio Frequency, Flexible, Triaxial, 95 ohms, M17/178-00001.
MIL-C-17/179 -	Cables, Radio Frequency, Flexible, Triaxial, 75 ohms, M17/179-00001.
MIL-C-17/180(EC) -	Cable, Radio Frequency, Flexible Coaxial, 75 ohms, M17/180-00001.
MIL-C-17/181(EC) -	Cables, Radio Frequency, Flexible Coaxial, 75 ohms, M17/181-00001 Unarmored, M17/181-00002 Armored.
MIL-C-17/182(EC) -	Cables, Radio Frequency, Flexible, Twin, 95 ohms, M17/182-00001 Unarmored, M17/182-00002 Armored.
MIL-C-17/183(EC) -	Cables, Radio Frequency, Flexible, Coaxial, 50 ohms, M17/183-00001.

MIL-C-17G
SUPPLEMENT 1

MIL-C-17/184(EC) - Cables, Radio Frequency, Flexible, Coaxial, 75 ohms, M17/184-00001.
MIL-C-17/185(EC) - Cables, Radio Frequency, Flexible, Coaxial, 93 ohms, M17/185-00001.
MIL-C-17/186(EC) - Cables, Radio Frequency, Flexible, Twin, 78 ohms, M17/186-00001.
MIL-C-17/187(EC) - Cables, Radio Frequency, Flexible, Coaxial, 50 ohms, M17/187-00001.
MIL-C-17/188(EC) - Cables, Radio Frequency, Flexible, Coaxial, 50 ohms, M17/188-00001.
MIL-C-17/189(EC) - Cables, Radio Frequency, Flexible, Coaxial, 50 ohms, M17/189-00001 Unarmored, M17/189-00002 Armored.
MIL-C-17/190(EC) - Cables, Radio Frequency, Flexible, Coaxial, 50 ohms, M17/190-00001.
MIL-C-17/191(EC) - Cable, Radio Frequency, Flexible, Coaxial, 75 ohms, M17/191-00001.
MIL-C-17/192(EC) - Cables, Radio Frequency, Flexible, Coaxial, 50 ohms, M17/192-00001.
MIL-C-17/193(EC) - Cables, Radio Frequency, Flexible, Coaxial, 50 ohms, M17/193-00001 Unarmored, M17/193-00002 Armored.
MIL-C-17/194(EC) - Cables, Radio Frequency, Flexible, Coaxial, 50 ohms, M17/194-00001.
MIL-C-17/195(EC) - Cables, Radio Frequency, Coaxial, 93 ohms, M17/195-00001.
MIL-C-17/196(EC) - Cables, Radio Frequency, Flexible, Coaxial, 50 ohms, M17/196-00001.
MIL-C-17/197(EC) - Cables, Radio Frequency, Flexible, Coaxial, 50 ohms, M17/197-00001.
MIL-C-17/198(EC) - Cables, Radio Frequency, Coaxial, 50 ohms, M17/198-00001.
MIL-C-17/199(EC) - Cables, Radio Frequency, Flexible, Coaxial, 50 ohms, M17/199-00001.
MIL-C-17/200(EC) - Cables, Radio Frequency, Flexible, Coaxial, 50 ohms, M17/200-00001.

RF Cable Selection Guide.

50 ohms, flexible, coaxial.

Part number	Overall diameter (OD)	Temp (°C)	Jacket	Frequency (GHz)	Notes
M17/93-RG178	.071 ±.004	-55 to +200	FEP	3	1/
M17/169-00001	.071 ±.004	-55 to +200	FEP		1/ 2/
M17/132-RG404	.071 ±.004	-55 to +200	FEP	3	Low noise 1/
M17/113-RG316	.098 ±.004	-55 to +200	FEP	3	1/
M17/172-00001	.098 ±.004	-55 to +200	FEP		1/ 2/
M17/138-00001	.098 ±.004	-55 to +200	PFA	3	1/
M17/119-RG174	.110 ±.004	-40 to +85	PVC	1	1/
M17/173-00001	.110 ±.004	-40 to +85	PVC		1/ 2/
M17/196-00001	.110 ±.005	-40 to +85	3/	1	1/
M17/152-00001	.114 ±.004	-55 to +200	FEP	12.4	1/
M17/54-RG122	.160 ±.005	-40 to +85	PVC	1	1/
M17/157-00001	.160 ±.005	-40 to +85	PVC		1/ 2/
M17/187-00001	.160 ±.005	-40 to +85	3/	1	1/
M17/198-00001	.160 ±.005	-40 to +85	3/		1/ 2/
M17/111-RG303	.170 ±.005	-55 to +200	FEP	3	4/
M17/170-00001	.170 ±.005	-55 to +200	FEP		2/ 4/
M17/028-RG058	.195 ±.004	-40 to +85	PVC	1	1/
M17/155-00001	.195 ±.004	-40 to +85	PVC		1/ 2/
M17/60-RG142	.195 ±.004	-55 to +200	FEP	12.4	4/

See footnotes at end of table.

MIL-C-17G
SUPPLEMENT 1

50 ohms, flexible, coaxial - Continued.

Part number	Overall diameter (OD)	Temp (°C)	Jacket	Frequency (GHz)	Notes
M17/158-00001	.195 ±.004	-55 to +200	FEP		2/ 4/
M17/128-RG400	.195 ±.004	-55 to +200	FEP	12.4	I/
M17/175-00001	.195 ±.004	-55 to +200	FEP		1/ 2/
M17/183-00001	.195 ±.004	-40 to +85	3/	1	I/
M17/197-00001	.195 ±.004	-40 to +85	3/		1/ 2/
M17/84-RG223	.212 ±.004	-40 to +85	PVC	12.4	4/
M17/167-00001	.212 ±.004	-40 to +85	PVC		2/ 4/
M17/194-00001	.212 ±.004	-40 to +85	3/	12.4	4/
M17/200-00001	.212 ±.004	-40 to +85	3/		2/ 4/
M17/112-RG304	.280 ±.005	-55 to +200	FEP	12.4	4/
M17/171-00001	.280 ±.005	-55 to +200	FEP		2/ 4/
M17/73-RG212	.332 ±.004	-40 to +85	PVC	11	4/
M17/162-00001	.332 ±.004	-40 to +85	PVC		2/ 4/
M17/188-00001	.332 ±.004	-40 to +85	3/	11	4/
M17/199-00001	.332 ±.004	-40 to +85	3/		2/ 4/
M17/127-RG393	.390 ±.010	-55 to +200	FEP	10	I/
M17/174-00001	.390 ±.010	-55 to +200	FEP		1/ 2/
M17/86-00001	.430 ±.010	-55 to +200	Fiberglass	10	I/ 5/
M17/87-00001	.500 ±.010	-55 to +200	Fiberglass	10	.198 OD I/ 5/ 6/ 7/
M17/74-RG213	.405 ±.007	-40 to +85	PVC	1	I/
M17/163-00001	.405 ±.007	-40 to +85	PVC		1/ 2/
M17/74-RG215	.405 ±.007	-40 to +85	PVC	1	.475 OD 3/ 5/
M17/189-00001	.405 ±.007	-40 to +85	3/	1	I/
M17/65-RG165	.410 ±.010	-55 to +250	Fiberglass	3	I/
M17/159-00001	.410 ±.010	-55 to +250	Fiberglass		1/ 2/
M17/65-RG166	.410 ±.010	-55 to +250	Fiberglass	3	.470 OD 1/ 7/
M17/92-RG115	.415 ±.015	-55 to +250	Fiberglass	12.4	1/
M17/168-00001	.415 ±.015	-55 to +250	Fiberglass		1/ 2/
M17/75-RG214	.425 ±.007	-40 to +85	PVC	11	I/
M17/164-00001	.425 ±.007	-40 to +85	PVC		1/ 2/
M17/190-00001	.425 ±.007	-40 to +85	3/	11	I/
M17/52-RG119	.465 ±.010	-55 to +200	Fiberglass	3	4/
M17/156-00001	.465 ±.010	-55 to +200	Fiberglass		4/ 2/
M17/52-RG120	.465 ±.010	-55 to +200	Fiberglass	3	.525 OD 4/ 7/
M17/78-RG217	.545 ±.010	-40 to +85	PVC	3	4/
M17/165-00001	.545 ±.010	-40 to +85	PVC		2/ 4/
M17/78-RG224	.545 ±.010	-40 to +85	PVC	3	.615 OD 4/ 5/ 6/ 7/
M17/192-00001	.545 ±.010	-40 to +85	3/	3	4/
M17/72-RG211	.730 ±.015	-55 to +200	Fiberglass	1	.47 5/
M17/161-00001	.730 ±.015	-55 to +200	Fiberglass		2/ 4/
M17/89-RG228	.730 ±.015	-55 to +200	Fiberglass	1	.795 OD 4/ 5/ 6/ 7/
M17/79-RG218	.870 ±.010	-40 to +85	PVC	1	4/
M17/166-00001	.870 ±.010	-40 to +85	PVC		2/ 4/
M17/79-RG219	.870 ±.010	-40 to +85	PVC	1	.945 OD 4/ 7/
M17/193-00001	.870 ±.010	-40 to +85	3/	1	4/
M17/67-RG177	.895 ±.015	-40 to +85	PVC	5.6	4/
M17/160-00001	.895 ±.015	-40 to +85	PVC		2/ 4/
M17/81-RG220	1.120 ±.015	-40 to +85	PVC	1	1/ 2/ 4/

- 1/ Stranded inner conductor.
- 2/ Non-swept cable.
- 3/ Cross-linked polyolefin.
- 4/ Solid inner conductor.
- 5/ To be revised.
- 6/ Inactive for new design.
- 7/ Armor.

MIL-C-17G
SUPPLEMENT 1

Cross-reference, swept cable to non-swept counterpart.

Swept	Non-swept
MIL-C-17/28	MIL-C-17/155
MIL-C-17/52	MIL-C-17/156
MIL-C-17/54	MIL-C-17/157
MIL-C-17/60	MIL-C-17/158
MIL-C-17/65	MIL-C-17/159
MIL-C-17/67	MIL-C-17/160
MIL-C-17/72	MIL-C-17/161
MIL-C-17/73	MIL-C-17/162
MIL-C-17/74	MIL-C-17/163
MIL-C-17/75	MIL-C-17/164
MIL-C-17/78	MIL-C-17/165
MIL-C-17/79	MIL-C-17/166
MIL-C-17/84	MIL-C-17/167
MIL-C-17/92	MIL-C-17/168
MIL-C-17/93	MIL-C-17/169
MIL-C-17/111	MIL-C-17/170
MIL-C-17/112	MIL-C-17/171
MIL-C-17/113	MIL-C-17/172
MIL-C-17/119	MIL-C-17/173
MIL-C-17/127	MIL-C-17/174
MIL-C-17/128	MIL-C-17/175
MIL-C-17/183	MIL-C-17/197
MIL-C-17/187	MIL-C-17/198
MIL-C-17/188	MIL-C-17/199
MIL-C-17/194	MIL-C-17/200

50 ohms, semirigid, coaxial.

Part number	Overall diameter (OD)	Temp (°C)	Jacket	Frequency (GHz)	Notes
M17/154-00001	.034 ±.001	-40 to +100	Copper	20	1/
M17/154-00002	.034 ±.002, -.001	-40 to +100	Copper	20	1/ 2/
M17/151-00001	.047 ±.001	-40 to +100	Copper	20	1/
M17/151-00002	.047 ±.002, -.001	-40 to +100	Copper	20	1/ 2/
M17/133-RG405	.086 ±.001	-40 to +100	Copper	20	17
M17/133-00001	.086 ±.002, -.001	-40 to +100	Copper	20	1/ 2/
M17/133-00002	.086 ±.001	-40 to +100	Copper	20	3/
M17/133-00003	.086 ±.002, -.001	-40 to +100	Copper	20	2/ 3/
M17/133-00004	.086 ±.001	-40 to +100	Copper	20	47
M17/133-00005	.086 ±.002, -.001	-40 to +100	Copper	20	2/ 4/
M17/130-RG402	.141 ±.001	-40 to +100	Copper	20	17
M17/130-00001	.141 ±.002, -.001	-40 to +100	Copper	20	1/ 2/
M17/130-00002	.141 ±.001	-40 to +100	Copper	20	47
M17/130-00003	.141 ±.002, -.001	-40 to +100	Copper	20	2/ 4/
M17/129-RG401	.250 ±.001	-40 to +125	Copper	18	17
M17/129-00001	.250 ±.002, -.001	-40 to +125	Copper	18	1/ 2/

1/ Silver copperweld center conductor.

2/ Tinned OD.

3/ Silver copper center conductor.

4/ Nickel-coated, copper-clad steel center conductor.

MIL-C-17G
SUPPLEMENT 1

75 ohms, coaxial.

Part number	Overall diameter (OD)	Temp (°C)	Jacket	Notes
M17/94-RG179	.100 ±.005	-55 to +200	FEP	1/ 2/
M17/110-RG302	.202 ±.005	-55 to +200	FEP	2/
M17/179-00001	.240 maximum	-55 to +150	Polyester braid	I/
M17/29-RG59	.242 ±.004	-40 to +85	PVC	2/
M17/184-00001	.242 ±.004	-40 to +85	4/	2/ 3/
M17/2-RG6	.332 ±.004	-40 to +85	PVC	3/
M17/180-00001	.332 ±.004	-40 to +85	4/	I/
M17/6-RG11	.405 ±.007	-40 to +85	PVC	4/
M17/181-00001	.405 ±.007	-40 to +85	4/	1/ 2/
M17/62-RG144	.410 ±.010	-55 to +200	Fiberglass	1/
M17/77-RG216	.425 ±.007	-40 to +85	PVC	3/
M17/191-00001	.425 ±.007	-40 to +85	4/	1/
M17/6-RG12	.475 maximum	-40 to +85	PVC (aluminum)	Armored M17/6-RG11 1/
M17/24-RG34	.630 ±.010	-40 to +85	PVC	1/
M17/64-RG164	.870 ±.010	-40 to +85	PVC	
M17/64-RG35	.945 maximum	-40 to +85	PVC (aluminum)	Armored M17/64-RG164
M17/40-RG85	.565 maximum	-40 to +85	PVC	

- 1/ Stranded center conductor.
2/ Copperweld.
3/ Double shield.
4/ Cross-linked polyolefin.

Various impedances, flexible, coaxial.

Part number	Ohms	Overall diameter (OD)	Jacket	Temp (°C)	Notes
M17/126-RG391	72 ±3	.405 ±.010	PVC	-40 to +85	1/ Low noise
M17/126-RG392	72 ±3	.475 maximum	PVC (aluminum)	-40 to +85	I/ 2/ Low noise
M17/095-RG180	95 ±5	.141 ±.004	FEP	-55 to +200	1/
M17/177-00001	95 ±5	.184 ±.004	FEP	-55 to +200	I/
M17/97-RG210	93 ±5	.242 ±.008	Fiberglass	-55 to +200	3/
M17/030-RG062	93 ±5	.242 ±.007	PVC	-40 to +85	3/
M17/185-00001	93 ±5	.242 ±.007	5/	-40 to +85	
M17/90-RG71	93 ±5	.245 ±.005	Polyethylene	-55 to +80	3/
M17/195-00001	93 ±5	.245 ±.005	5/	-40 to +85	
M17/178-00001	95 ±5	.305 maximum	Polyester braid	-55 to +150	1/
M17/100-RG133	95 ±5	.405 ±.010	PVC	-40 to +85	
M17/31-RG63	125 ±6	.405 ±.010	PVC	-40 to +85	3/
M17/31-RG79	125 ±6	.475 maximum	PVC (aluminum)	-40 to +85	3/ 4/
M17/47-RG114	185 ±10	.405 ±.010	PVC	-40 to +85	3/

- 1/ Stranded center conductor.
2/ Armored.
3/ Copperweld.
4/ Inactive for new design.
5/ Cross-linked polyolefin.

MIL-C-17G
SUPPLEMENT 1

Special application.

Part number	Application	Ohms	Overall diameter (OD)	Jacket	Temp (°C)	Notes
M17/45-RG108	Twin axial	78 ±7	.235 ±.010	PVC	-40 to +80	2/
M17/186-00001	Twin axial	78 ±7	.235 ±.010	1/	-40 to +80	2/
M17/182-00001	Twin axial	95 ±5	.420 ±.010	I/	-40 to +80	2/ Double shield
M17/56-RG130	Twin axial	95 ±5	.625 ±.015	PVC	-40 to +80	2/ 3/
M17/56-RG131	Twin axial	95 ±5	.710 maximum	PVC (aluminum)	-40 to +80	2/ 3/ 4/
M17/015-RG022	Twin axial	95 ±5	.420 ±.010	PVC	-40 to +80	3/ Double shield
M17/015-RG111	Twin axial	95 ±5	.490 maximum	PVC (aluminum)	-40 to +80	2/ 4/ Double shield
M17/16-RG23	Twin axial	125 ±5	.650 ±.020	PVC	-40 to +80	2/ Double shield each core shielded
M17/16-RG24	Twin axial	125 ±5	.735 maximum	PVC (aluminum)	-40 to +80	2/ 4/ Double shielded each core shielded
M17/34-RG65	Time delay	950 ±50	.405 ±.010	PVC	-40 to +80	5/
M17/176-00002	Twin axial	77 ±7	0.145	PFA	-55 to +200	2/ 6/

- 1/ Cross-linked polyolefin.
2/ Stranded center conductor.
3/ To be revised.
4/ Armored.
5/ Core center conductor.
6/ Data buss applications for MIL-STD-1760.

Pulse.

Part number	Ohms	O.D.	Jacket	Temp (°C)	Notes
M17/131-RG403	50 ±2	.116 ±.012	FEP	-55 to +200	4/ 2/ Triaxial
M17/116-RG307	75 ±4	.265 ±.005	Polyethylene	-55 to +80	4/ 2/ Triaxial
M17/21-RG26	48 ±4	.425 ±.015	Rubber	-40 to +80	1/ 3/
		.575 maximum	Aluminum	-40 to +80	
M17/33-RG64	48 ±4	.460 ±.015	Rubber	-40 to +80	4/ Double braid
M17/19-RG25	48 ±4	.505 ±.015	Rubber	-40 to +80	4/ Triaxial
M17/22-00001	48 ±4	.595 ±.015	Rubber	-40 to +80	4/
M17/22-RG27	48 ±4	.670 maximum	Aluminum	-40 to +80	4/ 3/
M17/125-RG329	50 ±4	.700 ±.020	Rubber	-40 to +80	4/ Triaxial
M17/23-RG28	48 ±4	.735 ±.020	Rubber	-40 to +80	4/ Triaxial
M17/124-RG328	25 ±2.5	1.460 ±.020	Polyethylene	-55 to +80	4/ 5/ Triaxial

- 1/ Stranded center conductor.
2/ Copperweld.
3/ Armored.
4/ Inactive for new design.
5/ Cord center conductor.

MIL-C-17G
SUPPLEMENT 1

Cross reference, PVC to polyolefin.

Cross-linked polyolefin	PVC jacket
MIL-C-17/180	MIL-C-17/2
MIL-C-17/181	MIL-C-17/6
MIL-C-17/182	MIL-C-17/15
MIL-C-17/183	MIL-C-17/28
MIL-C-17/184	MIL-C-17/29
MIL-C-17/185	MIL-C-17/30
MIL-C-17/186	MIL-C-17/45
MIL-C-17/187	MIL-C-17/54
MIL-C-17/188	MIL-C-17/73
MIL-C-17/189	MIL-C-17/74
MIL-C-17/190	MIL-C-17/75
MIL-C-17/191	MIL-C-17/77
MIL-C-17/192	MIL-C-17/78
MIL-C-17/193	MIL-C-17/79
MIL-C-17/194	MIL-C-17/84
MIL-C-17/195	MIL-C-17/90
MIL-C-17/196	MIL-C-17/119
MIL-C-17/197	MIL-C-17/155
MIL-C-17/198	MIL-C-17/157
MIL-C-17/199	MIL-C-17/162
MIL-C-17/200	MIL-C-17/167

RG cross reference.

RG number	Initial specification sheet number	Current specification sheet number or status	Connector accommodation series
5B	MIL-C-17/1	MIL-C-17/162	N, SC
6A	MIL-C-17/2		
8A	MIL-C-17/3	MIL-C-17/163	
9B	MIL-C-17/4	MIL-C-17/164	
10	MIL-C-17/5	MIL-C-17/74	N, C, SC
11	MIL-C-17/6		
12	MIL-C-17/7	MIL-C-17/6	
13	MIL-C-17/8	MIL-C-17/77	
14	MIL-C-17/9	MIL-C-17/165	MIL-C-3655 MIL-C-3655 MIL-C-3607 MIL-C-3607 MIL-C-3607
17	MIL-C-17/10	MIL-C-17/166	
18	MIL-C-17/11	MIL-C-17/166	
19	MIL-C-17/12	MIL-C-17/81	
20	MIL-C-17/13	MIL-C-17/81	
21	MIL-C-17/14	MIL-C-17/162	
22	MIL-C-17/15		
23	MIL-C-17/16		
24	MIL-C-17/17	MIL-C-17/16	
25	MIL-C-17/18	MIL-C-17/19	
26	MIL-C-17/20	MIL-C-17/21	
27	MIL-C-17/22		
28	MIL-C-17/23		
29		Canceled replaced by RG58	
34	MIL-C-17/24		
35	MIL-C-17/25	MIL-C-17/64	
55	MIL-C-17/26	MIL-C-17/167	

MIL-C-17G
SUPPLEMENT 1

RG cross reference - Continued.

RG number	Initial specification sheet number	Current specification sheet number or status	Connector accommodation series
57	MIL-C-17/27	MIL-C-17/56	
58	MIL-C-17/28	MIL-C-17/155	TNC, BNC, SMA
59	MIL-C-17/29		TNC, BNC, SMA
62A	MIL-C-17/30		TNC, BNC
62B	MIL-C-17/91 (USAF)	MIL-C-17/97	
63	MIL-C-17/31		N, C, SC
64	MIL-C-17/32	MIL-C-17/33	MIL-C-3607
65	MIL-C-17/34		TNC, BNC
71	MIL-C-17/90		
74A	MIL-C-17/35	MIL-C-17/165	
79	MIL-C-17/36	MIL-C-17/31	
81	MIL-C-17/37	Canceled	
82	MIL-C-17/38	Canceled	
84	MIL-C-17/39	Canceled	
85	MIL-C-17/40		
86	MIL-C-17/41	Canceled	
87A	MIL-C-17/42	MIL-C-17/86	
88	MIL-C-17/43	Inactive	
94	MIL-C-17/44	MIL-C-17/87	
108	MIL-C-17/45		MIL-C-3655
111	MIL-C-17/46	MIL-C-17/15	
114	MIL-C-17/47		N, C, SC
115	MIL-C-17/48	MIL-C-17/168	
116	MIL-C-17/49	MIL-C-17/86	
117	MIL-C-17/50	MIL-C-17/72	
118	MIL-C-17/51	MIL-C-17/161	
119	MIL-C-17/52	MIL-C-17/156	MIL-C-3643
120	MIL-C-17/53	MIL-C-17/52	
122	MIL-C-17/54	MIL-C-17/157	TNC, BNC, SMA
126	MIL-C-17/55	Canceled	
130	MIL-C-17/56		MIL-C-3655
131	MIL-C-17/57	MIL-C-17/56	
133	MIL-C-17/100		
140	MIL-C-17/58	MIL-C-17/110	
141	MIL-C-17/59	MIL-C-17/170	
142	MIL-C-17/60	MIL-C-17/158	TNC, BNC, SMA
143	MIL-C-17/61	MIL-C-17/112	
144	MIL-C-17/62		N, SC
146	MIL-C-17/63	Canceled	
149	MIL-C-17/117	MIL-C-17/126	
150	MIL-C-17/117	MIL-C-17/126	
151	MIL-L-3890/1		
152	MIL-L-3890/1		
153	MIL-L-3890/1		
154	MIL-L-3890/1		
155	MIL-L-3890/1		
156	MIL-C-17/101	Canceled	
157	MIL-C-17/102	Canceled	
158	MIL-C-17/103	Canceled	
161	MIL-C-17/118	Canceled	
164	MIL-C-17/64		
165	MIL-C-17/65	MIL-C-17/159	N, C, SC, HN
166	MIL-C-17/66	MIL-C-17/65	
174	MIL-C-17/119	MIL-C-17/173	SMA, SMB
176	MIL-C-17/120	Canceled	
177	MIL-C-17/67	MIL-C-17/160	N, HN
178	MIL-C-17/93	MIL-C-17/169	SMA, SMB, SMC

MIL-C-17G
SUPPLEMENT 1

RG cross reference - Continued.

RG number	Initial specification sheet number	Current specification sheet number or status	Connector accommodation series
179	MIL-C-17/94		SMA, SMB, SMC
180	MIL-C-17/95		TNC, BNC
181	MIL-C-17/104	Canceled	
187	MIL-C-17/68	MIL-C-17/94	
188	MIL-C-17/69	MIL-C-17/113	
190	MIL-C-17/105	Canceled	
191	MIL-C-17/106	Canceled	
195	MIL-C-17/70	MIL-C-17/95	
196	MIL-C-17/71	MIL-C-17/169	
209	MIL-C-17/96	Canceled	
210	MIL-C-17/97		TNC, BNC
211	MIL-C-17/72	MIL-C-17/161	C, SC, LT
212	MIL-C-17/73	MIL-C-17/162	N, C, SC
213	MIL-C-17/74	MIL-C-17/163	N, C, SC
214	MIL-C-17/75	MIL-C-17/164	N, C, SC
215	MIL-C-17/76	MIL-C-17/163	N
216	MIL-C-17/77		N
217	MIL-C-17/78	MIL-C-17/165	N, SC
218	MIL-C-17/79	MIL-C-17/166	N, C, SC, LC, LT
219	MIL-C-17/80	MIL-C-17/166	
220	MIL-C-17/81	Inactive	QL
221	MIL-C-17/82	MIL-C-17/81	
222	MIL-C-17/83	MIL-C-17/162	
223	MIL-C-17/84		TNC, BNC, SMA
224	MIL-C-17/85	MIL-C-17/165	
225	MIL-C-17/86		
226	MIL-C-17/87		
227	MIL-C-17/88	MIL-C-17/86	
228	MIL-C-17/89	MIL-C-17/161	
230	MIL-C-17/98 (USAF)	Canceled	
231	MIL-C-23806/1		
232	MIL-C-22931/11		
233	MIL-C-22931/13		
234	MIL-C-22931/15		
235	MIL-C-17/99	MIL-C-17/92	
236	MIL-C-22931/9		
237	MIL-C-22931/9		
240	MIL-C-22931/13		
242	MIL-C-22931/15		
244	MIL-C-22931/10		
245	MIL-C-22931/10		
246	MIL-C-22931/12		
247	MIL-C-22931/12		
248	MIL-C-22931/14		
249	MIL-C-22931/14		
250	MIL-C-22931/16		
251	MIL-C-22931/16		
252	MIL-C-22931/9		
253	MIL-C-22931/9		
254	MIL-C-22931/11		
255	MIL-C-22931/11		
257	MIL-C-22931/13		
258	MIL-C-22931/13		
264	MIL-C-23020/4		
265	MIL-C-22931/7		
266	MIL-C-17/122	Canceled	

MIL-C-17G
SUPPLEMENT 1

RG cross reference - Continued.

RG number	Initial specification sheet number	Current specification sheet number or status	Connector accommodation series
267	MIL-C-22931/6	MIL-C-22931/11	
268	MIL-C-22931/5	Canceled	
269	MIL-C-22931/11		
270	MIL-C-22931/13		
279	MIL-C-17/123	Canceled	
280	MIL-C-17/107	Canceled	
281	MIL-C-17/108	Canceled	
293	MIL-C-23020/1		
294	MIL-C-23020/2		
295	MIL-C-23020/3		
296	MIL-C-17/114	Canceled	
297	Drawing RE49C781		
298	MIL-C-22667		
299	Waveguide		
300	Waveguide		
301	MIL-C-17/109	Canceled	
302	MIL-C-17/110		TNC, BNC
303	MIL-C-17/111	MIL-C-17/170	TNC, BNC
304	MIL-C-17/112	MIL-C-17/171	TNC, BNC
305	Drawing RE496783 1/		
306	MIL-C-17/115	MIL-C-23806/2	
307	MIL-C-17/116		MIL-C-3607
308 - 315	MIL-R-9671		
316	MIL-C-17/113	MIL-C-17/172	SMA, SMB, SMC
317	MIL-C-23020/5		
318	MIL-C-22931/11		
319	MIL-C-22931/13		
320	MIL-W-85		
321	MIL-C-22931/15		
322	MIL-C-22931/15		
325		Canceled	
326	Drawing SC-DL-598921		
327		Canceled	
328	MIL-C-17/124		MIL-C-3607
329	MIL-C-17/125	Canceled	
330		Canceled	
331 - 336	MIL-C-23806/1 and 2		
337 - 359	MIL-W-85		
360	MIL-C-23806/3		
361	Drawing RE49D826		
363		Canceled	
364		Canceled	
365	SCL 6624/4		
366	Drawing RE49C828		
367	Drawing RE49C829		
369	MIL-C-22931		
370	MIL-C-22931		
375	Waveguide drawing RE49C833		
376 2/			
377	MIL-C-22931		
378	MIL-C-22931/13		
382	MIL-I-3890/3		

1/ Same as RG 290 except FEP.

2/ Same as RG 323 except corrugated aluminum outer conductor.

MIL-C-17G
SUPPLEMENT 1

RG cross reference - Continued.

RG number	Initial specification sheet number	Current specification sheet number or status	Connector accommodation series
385	MIL-C-22931/17		
388	MIL-C-23020		
389	DL-SC-B-459378		N, SC
391	MIL-C-17/126		
392	MIL-C-17/126		
393	MIL-C-17/127	MIL-C-17/174	N
396		Canceled	
399	MIL-C-22931/18		N, HN
400	MIL-C-17/128	MIL-C-17/175	TNC, BNC, SMA
401	MIL-C-17/129		TNC, N
402	MIL-C-17/130		SMA, TNC
403	MIL-C-17/131		
404	MIL-C-17/132		
405	MIL-C-17/133		SMA

Nato preferred cables.

NATO	Military pin	NATO	Military pin
NWR-1	M17/74-RG213	NWR-32	M17/113-RG316
NWR-2	M17/028-RG058	NWR-33	M17/094-RG179
NWR-3	M17/16-RG11	NWR-34	M17/93-RG178
NWR-4	M17/31-RG63	NWR-35	M17/75-RG214
NWR-5	M17/79-RG218	NWR-36	M17/86-00001
NWR-6	M17/64-RG164	NWR-45	M17/119-RG174
NWR-7	M17/100-RG133	NWR-46	M17/133-RG405
NWR-8	M17/33-RG65	NWR-47	M17/054-RG122
NWR-10	M17/65-RG165	NWR-48	M17/84-RG223
NWR-11	M17/29-RG59	NWR-49	M17/130-RG402
NWR-12	M17/030-RG062	NWR-50	M17/73-RG212
NWR-13	M17/72-RG211	NWR-51	M17/129-RG401
NWR-16	M17/62-RG144	NWR-52	M17/78-RG217
NWR-17	M17/74-RG215	NWR-53	M17/77-RG216
NWR-18	M17/6-RG12	NWR-54	M17/97-RG210
NWR-19	M17/79-RG219	NWR-55	M17/90-RG71
NWR-20	M17/64-RG35		
NWR-25	M17/60-RG142		
NWR-29	M17/124-RG328		
NWR-30	M17/111-RG303		
NWR-31	M17/110-RG302		

CONCLUDING MATERIAL

Preparing activity:
Army - CR

Agent:
DLA - ES

(Project 6145-1118)

MIL-C-17G
9 March 1990
SUPERSEDING
MIL-C-17F
18 January 1983

MILITARY SPECIFICATION

CABLES, RADIO FREQUENCY, FLEXIBLE AND SEMIRIGID,

GENERAL SPECIFICATION FOR

This specification is approved for use by all Departments and Agencies of the Department of Defense.

1. SCOPE

1.1 Scope. This specification covers flexible and semirigid cables with solid and semisolid dielectric cores, with single, dual and twin inner conductors. Cables covered by this specification are primarily intended for use as transmission lines to conduct energy in a simple power transfer continuously or intermittently. In general, these cables are designed for low-loss, stable operation from the relatively low frequencies through the higher frequencies in the microwave and radar regions of the frequency spectrum. Cables may also be used as circuit elements, delay lines or impedance matching devices. These cables are supplied under a reliability assurance program as specified in section 3.

1.2 Classification. Cables shall be the part number, as specified (see 3.1).

1.2.1 Cable types.

1.2.1.1 Flexible, coaxial single conductor. A flexible coaxial cable is constructed of a single inner conductor covered by a flexible low-loss r-f dielectric core material, which is then surrounded by a braided outer conductor(s), with the whole covered by a protective covering. In some cases this is covered by an extra braided armor for use in extremely abusive applications. Each element of the cable is designed to contribute to the requirements of the finished product.

1.2.1.2 Semirigid, coaxial single conductor. Semirigid coaxial cables are constructed of a single inner conductor covered by a flexible low-loss r-f dielectric core material, which is then surrounded by a solid, continuous, metallic outer conductor.

1.2.1.3 Two-conductor. Individual dielectric cores of two-conductor cables shall meet the requirements of solid or semisolid dielectric cores. One strand of one of the inner conductors shall be coded for identification and shall be visible without disturbing the stranding. That is, if all of the strands of the inner conductors are coated, then one strand shall be bare; or if all of the strands are bare, then one strand shall be coated.

Beneficial comments (recommendations, additions, deletions) and any pertinent data which may be used in improving this document should be addressed to: US Army Communications-Electronics Command, ATTN: AMSEL-ED-T0, Fort Monmouth, New Jersey 07703-5000 by using the self-addressed Standardization Document Improvement Proposal (DD Form 1426) appearing at the end of this document or by letter.
--

- a. Twin. Twin cables shall be constructed of individual inner conductors within individual dielectric cores, within a common outer conductor or may have individual inner conductors within a common outer core that may be filled-to-round.
- b. Dual. A dual cable shall be constructed of individual coaxial cables enclosed within a common outer conductor.

1.2.1.4 Triaxial. Triaxial cables are constructed the same as regular coaxial cables except for an additional interlayer of dielectric material over the outer conductor, over which is laid an extra shield, with the whole covered by a protective covering.

2. APPLICABLE DOCUMENTS

2.1 Government documents.

2.1.1 Specifications, standards, and handbooks. The following specifications, standards, and handbooks form a part of this document to the extent specified herein. Unless otherwise specified, the issues of these documents are those listed in the issue of the Department of Defense Index of Specifications and Standards (DODISS) and supplement thereto, cited in the solicitation (see 6.2).

SPECIFICATIONS

FEDERAL

L-P-389	- Plastic Molding Material, FEP Fluorocarbon, Molding and Extrusion.
L-P-390	- Plastic, Molding and Extrusion Material, Polyethylene and Copolymers (Low, Medium, and High Density).
QQ-R-175	- Resistance Wire.
TT-P-320	- Aluminum Pigment, Powder and Paste, For Paint.
TT-I-735	- Isopropyl Alcohol.
WW-T-700	- Tube, Aluminum Alloy, Drawn, Seamless; General Specification for.
WW-T-799	- Tube, Copper, Seamless, (For Use With Solder-flared- or Compression-Type Fittings).
UU-T-450	- Tissue, Facial.

MILITARY

MIL-I-631	- Insulation, Electrical, Synthetic-Resin Composition, Nonrigid.
MIL-Y-1140	- Yarn, Cord, Sleeving, Cloth and Tape-Glass.
MIL-I-3930	- Insulating and Jacketing Compounds, Electrical (For Cables, Cords, and Wires).
MIL-T-10727	- Tin Plating; Hot-Dipped, For Ferrous and Nonferrous Metals.
MIL-C-12000	- Cable, Cord, and Wire, Electric; Packaging of.
MIL-H-5606	- Hydraulic Fluid, Petroleum Base, Aircraft, Missile, and Ordnance
MIL-T-5624	- Turbine Fuel, Aviation, Grades JP-4 and JP-5.
MIL-F-16884	- Fuel, Naval Distillate.
MIL-L-17331	- Lubricating Oil, Steam Turbine and Gear, Moderate Service.
MIL-H-17672	- Hydraulic Fluid, Petroleum, Inhibited.
MIL-L-23699	- Lubricating Oil, Aircraft Turbine Engines, Synthetic Base.
MIL-L-24467	- Lubricating Oil, Steam Turbine, Vapor-Space Inhibited.
MIL-C-39012	- Connectors, Coaxial, Radio Frequency, General Specification for.

(See supplement 1 for list of applicable specification sheets.)

STANDARDS

FEDERAL

- FED-STD-228 - Federal Test Method No. 228, Cable and Wire, Insulated; Methods of Testing.
- FED-STD-601 - Federal Test Method No. 601, Rubber: Sampling and Testing.

MILITARY

- MIL-STD-105 - Sampling Procedures and Tables For Inspection By Attributes.
- MIL-STD-130 - Identification Marking Of US Military Property.
- MIL-STD-202 - Test Methods For Electronic and Electrical Component Parts.
- MIL-STD-384 - Radio Frequency Connector Interfaces for,
- MIL-STD-45662 - Calibration Systems Requirements.

(Unless otherwise indicated, copies of federal and military specifications, standards, and handbooks are available from the Naval Publications and Forms Center, (ATTN: NPODS), 5801 Tabor Avenue, Philadelphia, PA 19120-5099.)

2.1.2 Other Government documents, drawings, and publications. The following other Government documents, drawings, and publications form a part of this document to the extent specified herein. Unless otherwise specified, the issues are those cited in the solicitation.

NAVAL ENGINEERING STANDARDS (NES)

- 711 - Determination of the Smoke Index of the Products of Combustion from Small Specimens of Materials.
- 713 - Determination of the Toxicity Index of the Products of Combustion from Small Specimens of Materials.

(Copies of Naval Engineering Standards are sponsored by the Procurement Executive, Ministry of Defense, ship department, section TE112, block G, Foxhill, Bath SA8 England.)

2.2 Non-Government publications. The following documents form a part of this document to the extent specified herein. Unless otherwise specified, the issues of the documents which are DoD adopted are those listed in the issue of the DODISS cited in the solicitation. Unless otherwise specified, the issues of documents not listed in the DODISS are the issues of the documents cited in the solicitation (see 6.2).

AMERICAN SOCIETY FOR TESTING MATERIALS:

- ASTM A-411 - Galvanized, Zinc-Coated, Low-Carbon Steel, Armor Wire.
- ASTM B-3 - Soft or Annealed, Copper Wire.
- ASTM B-8 - Concentric-Lay-Stranded, Copper Conductors.
- ASTM B-33 - Tin-coated, Soft or Annealed, Copper Wire.
- ASTM B-197 - Copper-Beryllium Alloy Wire.
- ASTM B-211 - Aluminum, Alloy Bars, Rods and Wire.
- ASTM B-286 - Copper Conductors for Use in Hookup Wire for Electronic Equipment.
- ASTM B-298 - Silver-Coated, Soft or Annealed, Copper Wire.
- ASTM B-344 - Nickel-Chromium and Nickel-Chromium-Iron Alloy, For Electrical Heating Elements.

- ASTM B-447 - Standard Specification for Welded Copper Tube.
- ASTM B-452 - Copper-Clad Steel Wire for Electronic Application.
- ASTM B-501 - Silver-Coated Copper-Clad Steel Wire for Electronic Applications.
- ASTM B-566 - Copper-Clad Aluminum Wire.
- ASTM D-470 - Test Of Rubber and Thermoplastic Insulated Wire and Cable.
- ASTM D-1352 - Ozone-Resisting Butyl Rubber Insulation For Wire and Cable.
- ASTM D-1457 - Materials, PTFE Molding and Extrusion.
- ASTM D-3159 - ETFE Fluoroplastic Molding and Extrusion Materials.
- ASTM D-3275 - E-CTFE Fluoroplastic Molding, Extrusion and Coating Materials.
- ASTM D-3307 - PFA - Fluorocarbon Molding and Extrusion Materials.
- ASTM B-355 - Nickel-Coated Soft or Annealed Copper Wire.
- ASTM D-2240 - Rubber Property-Durometer Hardness. (DOD adopted)
- ASTM D-2565 - Standard Practice for Operating Xenon Arc-Type (Water-Cooled) Light-Exposure Apparatus Wire and Without Water for Exposure of Plastics.
- ASTM D-4245 - Standard Specification for Ozone-Resistant Thermoplastic Elastomer Insulation for Wire and Cable.

(Applications for copies should be addressed to the American Society For Testing Materials, 1916 Race Street, Philadelphia, PA 19103-1137.)

INSTITUTE OF ELECTRICAL AND ELECTRONIC ENGINEERS

- IEEE-STD-383 - IEEE Standard for Type of Class IE Electric Cable, Field Splices, and Connections for Nuclear Power Generating Stations.
- IEEE-STD-287 - Standard for Precision Coax Connectors.

(Applications for copies should be addressed to the The Institute of Electrical and Electronic Engineers, Inc., 345 East 47th Street, New York, NY 10017).

(Non-Government standards and other publications are normally available from the organizations that prepare or distribute the documents. These documents also may be available in or through libraries or other informational services.)

2.3 Order of precedence. In the event of a conflict between the text of this document and the references cited herein (except for related associated detail specifications, specification sheets, or MS standards), the text of this document shall take precedence. Nothing in this document, however, supersedes applicable laws and regulations unless a specific exemption has been obtained.

3. REQUIREMENTS

3.1 Specification sheets. The individual item requirements shall be as specified herein and in accordance with the applicable specification sheets. In the event of any conflict between the references of this specification and the specification sheet, the latter shall govern.

3.2 Classification of requirements. The classification of requirements for cables are as follows:

TABLE 1. Classification of requirements.

Requirements	Paragraph
Qualification	3.3
Materials	3.4
Design and construction	3.5
Visual and mechanical	3.6
Operational	3.7
Marking	3.8
Weight	3.9
Workmanship	3.10

3.3 Qualification. Cable furnished under this specification shall be products which are qualified for listing on the applicable qualified products list at the time set for opening of the bids (see 4.6 and 6.3).

3.3.1 Reliability. The contractor's reliability program for manufactured cable and manufacturing procedures shall conform to 4.1.3 and shall be effective 12 months from the date of MIL-C-17G.

3.4 Materials. Unless otherwise specified (see 3.1), the materials for the principal components of the cable shall be as specified herein. Prior approval to use substitute material must be obtained from the qualifying activity. When a definite material is not specified, a material shall be used that will enable the finished products to meet the performance requirements of this specification. Acceptance or approval of any constituent material shall not be construed as a guaranty of the acceptance of the finished product.

3.5 Design and construction. Unless otherwise specified (see 3.1), cables shall be of the design and construction specified herein.

3.5.1 Inner conductors. The inner conductor shall be solid, stranded, braided or helical, bare or coated, as specified (see 3.1). The materials and coatings shall be as specified (see 3.1).

3.5.1.1 Solid inner conductors:

- a. Bare copper wire. Bare copper wire shall conform to soft or annealed copper wire in accordance with ASTM B-3.
- b. Tin-coated copper wire. Tin-coated copper wire shall conform to tin-coated, soft or annealed copper wire in accordance with ASTM B-33.
- c. Silver-coated copper wire. Silver-coated copper wire shall conform to ASTM B-298, except thickness of silver coating shall not be less than 40 microinches.
- d. Copper-clad steel wire. Copper-clad steel wire shall conform to high-strength, 40 percent conductivity, hard-drawn, copper-clad, steel wire in accordance with ASTM B-452, class 40HS.
- e. Annealed copper-clad steel wire. Annealed copper-clad steel wire shall have the same requirements as for copper-clad steel wire specified in 3.5.1.1(d), except shall be annealed. The tensile strength shall be 50,000 lbf/in² minimum.
- f. Silver-coated copper-clad steel wire. Silver-coated copper-clad steel wire shall conform to ASTM B-501, class 40 HS or 40A, except thickness of silver coating shall not be less than 40 microinches.
- g. Annealed copper-clad aluminum wire. Annealed copper-clad aluminum wire shall conform to ASTM B-566, class 10A or 15A. The thickness of the copper covering shall be 3.5 percent minimum of the wire radius (8 to 12 percent by volume) for class 10A, and 5 percent minimum of the wire radius (13 to 17 percent by volume) for class 15A.
- h. Copper-beryllium alloy wire. Copper-beryllium alloy wire shall conform to solution-heat-treated, half-hard wire in accordance with ASTM B-197, Alloy 172. The tensile strength shall be 110,000 to 135,000 lbf/in².

- i. Annealed-copper-beryllium wire. Same as (h) above except the tensile strength shall be 80,000 lbf/in².
- j. Silver-coated wire. Silver-coating over other wire material shall conform to ASTM B-298 with proper correction for the density of the base material when the gravimetric reference procedure is used.
- k. High resistance wire. High resistance wire shall conform to QQ-R-175, composition E (80 percent nickel - 20 percent chromium). The tensile strength shall be 100,000 lbf/in² minimum. The resistance change with temperature shall be in accordance with ASTM B-344.

3.5.1.2 Stranded inner conductors. Stranded inner conductors shall be concentrically stranded in accordance with ASTM B-8 or ASTM B-286. Tensile strength and elongation of conductors shall be tested prior to stranding. Conductors shall not be coated after stranding (no overcoating). Individual wires, before stranding, shall meet all the requirements of the basic wires specified in 3.5.1.1. Diameter tolerances for the completed inner conductor shall be rounded to the next highest .001 inch.

3.5.1.3 Conductor joints. Joints in individual strands of a stranded wire shall not be closer together than 5 lay-lengths.

3.5.2 Dielectric cores. The material used in the dielectric cores specified (see 3.1) shall be of uniform thickness consistent with the electrical, environmental, physical, mechanical and dimensional requirements.

- a. Solid dielectric cores. Solid dielectric cores shall be extruded or tape-wrapped as specified (see 3.1) and talc-coated when specified (see 3.1).
- b. Semisolid (air-spaced) dielectric cores. Semisolid, air-spaced dielectric cores shall be constructed in such a manner that air spaces are a basic element of the construction.

3.5.2.1 Dielectric core types. The material for the dielectric cores shall be one of the following specified types (see 3.1). The dielectric constant and the dissipation factor shall be consistent with the applicable electrical requirements.

- a. Type A. Polyethylene (PE) conforming to L-P-390, type II, class I, grade 3, low-density type.
- b. Type A-1. Solid polyethylene.
- c. Type A-2. Solid polyethylene coated with the best commercial grade of talc, to prevent sticking between individual components of the cable.
- d. Type A-3. Air-spaced polyethylene. One polyethylene filament thread or a braid of more than one filament threads within a tube of solid polyethylene, or spiraled fins of polyethylene between tubes of solid polyethylene.
- e. Type A-4. Air-spaced polyethylene. Foamed polyethylene.
- f. Type A-5. Conductive polyethylene shall conform to L-P-390, type III, carbon-black type. The maximum resistance per foot shall be as specified (see 3.1).

- g. Type D. (Not for future design). Dielectric core shall be a composite of three layers of dielectric materials. Each layer shall make intimate contact with each other, except that the outer layer shall be easily strippable.
- Inner layer. Type H, semiconducting synthetic rubber (see 3.5.2.1(r)).
- Middle layer. Type W, insulating synthetic rubber (see 3.5.2.1(x)).
- Outer layer. Type H, semiconducting synthetic rubber (see 3.5.2.1(r)).
- h. Type E. (Not for future design). Same as type D except outer layer shall be type Q (insulated polychloroprene rubber) which need not be easily strippable.
- i. Type F. Polytetrafluoroethylene (PTFE) shall conform to ASTM D1457.
- j. Type F-1. Solid, extruded PTFE.
- k. Type F-2. Solid PTFE tape wrapped.
- l. Type F-3. Air-spaced PTFE perforated tape wrapped.
- m. Type F-4. Air-spaced PTFE. One PTFE filament thread or a braid of more than one PTFE filament thread within a tube of tape-wrapped PTFE.
- n. Type F-5. Air-spaced PTFE, porous tape wrapped.
- o. Type F-6. Air-spaced PTFE, expanded tape wrapped.
- p. Type F-7. Solid PTFE, coated with a semiconducting material.
- q. Type G. (Not for future design). Solid mineral material (such as magnesium oxide) consisting of finely divided particles free from detrimental impurities which shall be packed tightly under high pressure.
- r. Type H. (Not for future design). Semiconducting synthetic rubber. The volume resistivity of this compound shall be within the range of 100 to 1,000 ohm-cm when tested in accordance with method 9111 in accordance with FED-STD-601, and colored black.
- s. Type J. Insulating synthetic butyl rubber. Butyl rubber shall be a copolymer of isobutylene and isoprene in accordance with ASTM D-1352, table I, colored gray.
- t. Type M. Fluorinated ethylene propylene (FEP) conforming to L-P-389, type I.
- u. Type M-1. Solid, extruded FEP.
- v. Type M-2. Air-spaced FEP. Foamed FEP.
- w. Type Q. (Not for future design). Insulating polychloroprene rubber, and colored red.
- x. Type W. (Not for future design). Insulating synthetic rubber. The material shall have a tensile strength of 500 lbf/in² minimum and an elongation of 300 percent minimum in 10 inches in accordance with ASTM D-470.

3.5.3 Outer conductors or extra shields. Outer conductors or extra shields shall be braided or solid (tubular), as specified (see 3.1).

3.5.3.1 Braided outer conductors or shields. Braids shall be applied with the maximum tension possible so as to prevent loosening or creeping but not to cause broken ends. Braids shall have no gaps. Loose strand ends shall be trimmed to within 1/32 inch of the braid and shall lay parallel with the braid. There shall be no splices of the completed braid. The number of braids and the elements of their construction shall be as specified (see 3.1). The individual strands of the braid shall meet the applicable requirements of the basic wires specified in 3.5.1.1. Strands may also be made of galvanized steel wires (see 3.5.3.1.1). The percent coverage specified (see 3.1) shall be determined in accordance with the formulas shown below.

$$\text{Percent coverage} = (2F - F^2) \times 100\%; \quad F = \frac{N P d}{\sin a}; \quad a = \tan^{-1} \left(\frac{2\pi (D + 2d) P}{C} \right)$$

Where: D = Maximum outside diameter of the dielectric core under the braid. In the case of double braid construction, the diameter (D) for determining the coverage of the outside braid shall be the outside diameter of the inner braid.

d = Diameter of an individual strand of the braid.

N = Number of ends (wire strands) per carrier.

C = Number of carriers (separated group of ends) around the diameter of the cable.

P = Minimum number of picks per inch (separation points between carriers) along the length of the cable.

a = Smaller angle between longitudinal axis of the cable and the braid wires.

F = Fill or space factor.

For two-conductor cables that are not filled-to-round and not twisted.

$$a = \tan^{-1} \left(\frac{2\pi (D_1 + 2d) P}{C} + \frac{4(D_2 - D_1) P}{C} \right)$$

Where: D₁ = Same as D above, except the minor diameter.

D₂ = Same as D above, except the major diameter.

3.5.3.1.1 Galvanized steel wire braids. When galvanized steel wire braids are specified (see 3.1), the individual strands shall be soft or annealed, low-carbon, steel wires in accordance with ASTM A-411. The tensile strength of the individual strands shall be 50,000 lbf/in² minimum. Tin plate (hot-dipped) in accordance with MIL-T-10727, type II may be used as an alternate to galvanize.

3.5.3.2 Solid (tubular) outer conductors. Solid outer conductors shall be constructed of metallic tubing, annealed before the final sink.

- a. Copper-tubing outer conductors. Copper tubing shall be 99 percent minimum purity. Seamless copper tubing in accordance with WW-T-799. Welded copper tubing in accordance with ASTM B-447, fully finished tube with IFR flash removal. The welded copper tubing shall be cold worked and re-crystallized to a uniform grain size throughout the structure with no evidence of the original weld.

- b. Aluminum-tubing outer conductors. Seamless, aluminum tubing shall be 99 percent minimum purity in accordance with WW-T-700.
- c. Solid outer conductor joints. Joints shall be within the specified dimensions and tensile strength limits specified for the basic solid outer conductor.

3.5.4 Barrier tapes. When specified (see 3.1), the barrier tapes shall be applied tightly and ride smoothly over the outer conductor. The barrier tape material shall be of the following type:

Type FF-2. PTFE tape wrapped. The PTFE may be reclaimed material. Unless otherwise specified (see 3.1), the tapes shall overlap 50 percent of the width of the tapes.

3.5.5 Interlayers. When specified (see 3.1), the interlayer shall be applied tightly and ride smoothly over the outer conductor. The interlayer material shall be one of the following types:

- a. Type A-1R. Polyethylene conforming to L-P-390, type II, class L, grade 4, low-density type, and colored red.
- b. Type C-1. (Not for future design). Braid of cotton tapes of 30 denier/2 ply.
- c. Type K. Polyethylene-terephthalate tape conforming to MIL-I-631, type G, form T, subform T, class I, fungus-resistant type. Unless otherwise specified (see 3.1), the tapes shall overlap 50 percent minimum of the width of the tapes.
- d. Type L. (Not for future design). Glass fiber tapes filled with, and uniformly coated with, silicone rubber on both sides and properly cured. Curing may be accomplished after applying the tapes to the conductor. The tapes shall be held from unwinding by being selfbonding, by using a silicone rubber adhesive or by means of a binder over the insulating tapes.
- e. Type U-1. (Not for future design). Urethane elastomer tape.
- f. Type R-1. (Not for future design). Rubber-filled tape.

3.5.6 Jackets. The jacket material shall be tough, flexible and nonhygroscopic. The jacket shall cover the cable tightly and evenly in a manner consistent with the physical, mechanical, environmental and dimensional requirements. Color shown is for outer surface of jacket. The jacket material shall be one of the following types unless otherwise specified (see 3.1):

- a. Type IIa. Noncontaminating type of medium-low-temperature, plasticized or compounded, polyvinylchloride or polyvinylchloride-acetate in accordance with MIL-I-3930, type JP, and colored black.
- b. Type IIIa. (Not for future design). Polyethylene conforming to L-P-390, type III, class L, grade 2, weather-resistant type, and colored black.
- c. Type IV. Polychloroprene rubber, medium-low-temperature type conforming to MIL-I-3930, type JN, and colored black.
- d. Type V. Fiberglass braids of the number specified (see 3.1). The braids shall be impregnated with a silicone-base varnish, and oven-baked. The glass fibers shall conform to MIL-Y-1140, class C, and colored brown.

- e. Type VI. (Not for future design). Silicone-rubber-polyester fiber construction. The inner element shall be a single braid of fiberglass impregnated with a silicone-base varnish, under an extruded or tape-wrapped layer of silicone rubber, and the whole thoroughly cured. As an alternate, the inner construction may be a wrap(s) of silicone rubber impregnated fiberglass tape, which shall be fused during processing. Over either construction there shall be a protective braid of polyester fiber impregnated with a high-temperature fluorocarbon lacquer, and colored orange.
- f. Type VII. Polytetrafluoroethylene (PTFE) shall conform to ASTM D-1457, and colored white.
- g. Type VIIa. Extruded PTFE.
- h. Type VIIb. PTFE tape wrapped. There shall be two wraps of unsintered tapes applied in opposite directions with an overlap of 50 percent minimum of the width of the tapes, and the whole fused during processing.
- i. Type VIII. (Not for future design). Polychloroprene rubber, low-temperature type conforming to MIL-I-3930, type JN-L, and colored black.
- j. Type IX. Extruded fluorinated ethylene propylene (FEP) transparent enough to permit the reading of marking tape through the jacket.
- k. Type X. Extruded copolymer of ethylene and tetrafluoroethylene (ETFE) in accordance with ASTM D-3159.
- l. Type XI. Extruded copolymer of ethylene and chlorotrifluoroethylene (E-CTFE) type III in accordance with ASTM D-3275.
- m. Type XII. Low-temperature, heat and weather resistant polyurethane thermoplastic elastomer in accordance with MIL-I-3930.
- n. Type XIII. Perfluoroalkoxy (PFA) in accordance with ASTM D-3307, type 1 having a tensile strength of 3,000 lbf/in² and a minimum elongation of 275 percent.
- o. Type XIV. Cross-linked polyolefin.
- p. Type XV. Styrene block copolymer or equivalent thermoplastic elastomer (TPE) in accordance with ASTM D-4245.

3.5.7 Armor. Metal armoring shall be of a braid construction that is rugged, tough, and flexible.

- a. Braid. Individual braid wires shall be No. Alclad 5056 aluminum-alloy in accordance with ASTM B-211. The diameter shall be .0126 $\pm$.0005 inch and the tensile strength shall be 52,000 lbf/in² minimum, before application onto the cable. The percent coverage shall be 88 percent minimum. The formulas shown in 3.5.3.1 shall be used to determine the percent coverage of the braid construction.
- b. Paint. Armor shall be covered with an aluminum paint conforming to TT-P-320, paste form, and colored light green.

3.6 Visual and mechanical inspection. When cables are examined and tested as specified in 4.8.1, the visual and mechanical characteristics shall be as specified (see 3.1).

3.6.1 Diameter measurements. When cables are examined as specified in 4.8.1.1, the diameter measurements shall be as specified (see 3.1).

3.6.2 Out-of-roundness of jacket measurements (when specified, see 3.1). When cables are examined as specified in 4.8.1.2, the out-of-roundness of the jacket diameter dimensions shall be as specified (see 3.1).

The dimensions shall be as specified in the detailed specification and out-of-roundness (the difference in diameter dimension in mutual perpendicular planes at any cross section) shall not exceed 50 percent of the difference between minimum and maximum diameters specified.

3.6.3 Eccentricity of inner conductor (not applicable to cables that have the inner conductor formed over an inner conductor support). When cables are examined as specified in 4.8.1.3, the displacement of the inner conductor shall not exceed 10 percent of the core radius, unless otherwise specified (see 3.1).

3.6.4 Adhesion of conductors. When cables are tested as specified in 4.8.1.4, the adhesion of the inner conductor to the dielectric core and the adhesion of the dielectric core to the outer conductor shall be as specified (see 3.1).

3.7 Operational. Unless otherwise specified (see 3.1), the operational requirements shall be as specified herein.

3.7.1 Continuity. When cables are tested as specified in 4.8.2, each conductor and shield shall be continuous.

3.7.2 Spark test (not applicable to semirigid cables or to cables with type V and type VI jackets). When cables are tested as specified in 4.8.3, there shall be no breakdown, flashover, or sparkover.

3.7.3 Voltage withstanding. When cables are tested as specified in 4.8.4, there shall be no breakdown, flashover, or sparkover.

3.7.4 Insulation resistance. When cables are tested as specified in 4.8.5, the insulation resistance per 1,000 feet shall be as specified (see 3.1).

3.7.5 Corona extinction voltage. When cable test specimens are tested as specified in 4.8.6 the corona extinction voltage shall be no less than that specified (see 3.1).

3.7.6 Characteristic impedance. When cables are tested as specified in 4.8.7, the maximum characteristic impedance shall not exceed the higher value specified, and the minimum shall not be less than the lower value specified (see 3.1).

3.7.7 RF transmission loss (attenuation). When cables are tested as specified in 4.8.8, the RF transmission loss shall not exceed the values specified over the frequency range or at the frequencies specified (see 3.1).

3.7.8 Standing wave ratio (return loss). When cables are tested as specified in 4.8.9 the standing wave ratio (return loss) shall be within the specified limits over the specified frequency range (see 3.1).

3.7.9 Capacitance. When cables are tested as specified in 4.8.10, the maximum capacitance shall be as specified (see 3.1).

3.7.10 Capacitance stability. When cables are tested as specified in 4.8.11, the capacitance during and after the test shall not have changed from its initial measurement more than the specified value (see 3.1).

3.7.11 Capacitance unbalance (for two-conductor cables only). When cables are tested as specified in 4.8.12, the capacitance unbalance shall not exceed the specified value (see 3.1).

3.7.12 Transmission unbalance (for two-conductor cables only). When cables are tested as specified in 4.8.13, the transmission unbalance shall not exceed the specified value (see 3.1).

3.7.13 Mechanically induced noise voltage (for low noise cables only). When cables are tested as specified in 4.8.14, the mechanically induced noise voltage shall not exceed the specified value (see 3.1).

3.7.14 Time delay. When cables are tested as specified in 4.8.15, the time delay shall be as specified (see 3.1).

3.7.15 Aging stability (not applicable to semirigid or cables with type IX jackets). When cables are tested as specified in 4.8.16, there shall be no evidence of cracks, flaws, or other damage in the jacket material.

3.7.16 Stress-crack resistance (FEP jacket). Unless otherwise specified (see 3.1), cable shall be tested as specified in 4.8.17. There shall be no evidence of cracks, flaws or other damage in the jacket material.

3.7.17 Outer conductor integrity (only semirigid cables). When cables are tested as specified in 4.8.18, there shall be no evidence of cracks, flaws, or other damage in the outer conductor material.

3.7.18 Cold bend (not applicable to semirigid cables). When cables are tested as specified in 4.8.19, there shall be no evidence of cracks, flaws, or other damage in the jacket material of flexible cables or the dielectric core material of flexible cable.

3.7.19 Dimensional stability (not applicable to time delay cable and cables with braided inner conductor). When cables are tested as specified in 4.8.20, the measurement at each end shall not exceed the specified value (see 3.1).

3.7.20 Contamination (PVC type IIa jacket cable only). When cables are tested as specified in 4.8.21, the delta Q shall not exceed 2.5.

3.7.21 Bendability (semirigid only). When cables are tested as specified in 4.8.22, there shall be no cracks, splits, fracturing, wrinkling, or other damage in the solid outer conductor material, after being formed around the mandrel diameter specified (see 3.1).

3.7.22 Flammability (when specified (see 3.1)). When cables are tested as specified in 4.8.23, the rate of travel of the flame shall not exceed 1 inch per minute and cable surface shall not flame for more than 1 minute after the gas flame is withdrawn. There shall be no flaming of the tissue as a result of incendiary drippings from the specimen.

3.7.23 Flame propagation (when specified (see 3.1)). Samples of completed cable, when tested in accordance with 4.8.25, shall be self-extinguishing and shall not burn to the top of the tray.

3.7.24 Acid gas generation. When cables are tested as specified in 4.8.26, the acid equivalent shall not exceed the percentage, by weight of the sample, as specified (see 3.1).

3.7.25 Halogen content. When cables are tested as specified in 4.8.27, the halogen content shall not be greater than specified (see 3.1).

3.7.26 Immersion tests. When cables are tested as specified in 4.8.28, the tensile strength and elongation shall be no less than that specified (see 3.1) and there shall be no evidence of cracks, flaws, or other damage to the jacket material.

3.7.27 Smoke index. When cables are tested as specified in 4.8.29, the smoke index shall not be greater than that specified (see 3.1).

3.7.28 Toxicity index. When cables are tested as specified in 4.8.30, the toxicity index shall not be greater than that specified (see 3.1).

3.7.29 Durometer hardness. When cables are tested as specified in 4.8.31, the hardness shall be as specified (see 3.1).

3.7.30 Weathering. When cables are tested as specified in 4.8.32, the tensile strength and elongation shall be no less than 75 percent of their unweathered values (see 3.1). The surface shall exhibit no signs of cracking when examined using 3X magnification.

3.7.31 Abrasion resistance. When tested as specified in 4.8.33, failure shall be construed if electrical contact occurs between either abrading element and the specimen conductor (as evidenced by cessation of cylinder rotation) prior to completing the specified number of abrasive scrapes (see 3.1). Test must be conducted on no fewer than 5 specimens.

3.7.32 Tear strength. When tested as specified in 4.8.34, the percentage heat distortion shall be no greater than that specified (see 3.1). Test must be conducted on no fewer than 6 specimens.

3.7.33 Heat distortion. When tested as specified in 4.8.35, the percentage heat distortion shall be no greater than that specified (see 3.1).

3.7.34 Physicals (aged). When tested as specified in 4.8.36, the specimens tensile strength and elongation shall not be less than that specified (see 3.1).

3.7.35 Tensile strength and elongation (unaged). When tested as specified in 4.8.37, the cable jacket shall have a tensile strength and elongation no less than that specified (see 3.1).

3.8 Marking. Cables shall be marked with the part number, military specification number, manufacturer's code symbol and name, in accordance with the basic requirements of MIL-STD-130. The marking shall be done in such a manner as not to permanently indent, deform or otherwise damage the jacket or outer covering. The marking shall be visible and legible from the outside of the cable, except for armored cables. The marking shall be legible after the aging stability and stress crack resistance tests. The following details shall apply:

- a. Armored cables. Armored cables shall be marked at intervals not exceeding 6 inches by inserting a suitably printed tape under the armor or jacket providing the marking is legible after the cable construction is completed. When the armor is added to a cable that has been previously marked with its unarmored type designation, the marking tape shall be inserted between the armor and the jacket only. When cables are so double marked, the marking on or under the jacket shall be disregarded.
- b. Unarmored cables.
 - (1) Types IIa, IIIa, IV, VI, VIII, XIV and XV jackets shall be surface marked at intervals not exceeding 2 feet. Cables with type V jackets shall be marked with tapes or surface marked in ink. Cables with type VI, X, and XI jackets may be optionally marked with tapes in lieu of ink.
 - (2) Types IX and XIII jackets shall be marked at intervals not exceeding 6 inches with marker tape or surface marking. For cables (types IX and XIII jackets) having a nominal outside diameter of .150 inch or less the method of marking shall be at the manufacturer's discretion, but with the qualifying activities approval and the marking as minimum must reflect the manufacturer's CAGE code.

- (3) Cables, twin axial, which do not have a requirement for fill-to-round, may be marked with a tape under the jacket regardless of jacket type.

c. Semirigid cables and unarmored cables with type VII jackets need not be marked.

3.9 Weight. When cables are tested as specified in 4.8.24, the maximum weight of completed cable construction shall be as specified (see 3.1).

3.10 Workmanship. All cables shall be manufactured and processed in such a manner as to be uniform in quality and shall be free from any burrs, die marks, chatter marks, foreign material and other defects that will affect life, serviceability, or appearance. Workmanship shall be such as to enable the cable to meet the applicable requirements of this specification.

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any other facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

4.1.1 Responsibility for compliance. All items shall meet all requirements of sections 3 and 5. The inspection set forth in this specification shall become a part of the contractor's overall inspection system or quality program. The absence of any inspection requirements in the specification shall not relieve the contractor of the responsibility of ensuring that all products or supplies submitted to the Government for acceptance comply with all requirements of the contract. Sampling inspection, as part of manufacturing operations, is an acceptable practice to ascertain conformance to requirements, however this does not authorize submission of known defective material, either indicated or actual, nor does it commit the Government to accept defective material.

4.1.2 Test equipment and inspection facilities. Test and measuring equipment and inspection facilities of sufficient accuracy, quality, and quantity to permit performance of the required inspection shall be established and maintained by the contractor. The establishment and maintenance of a calibration system to control the accuracy of the measuring and test equipment shall be in accordance with MIL-STD-45662.

4.1.3 Reliability assurance program. A reliability assurance program shall be established and maintained. Process control records shall cover the implementation of devices such as control charts (e.g., $\bar{X}$ bar and R charts) or other means of indication of the degree of control achieved in the production process. Records shall also indicate the action taken when each out-of-control condition is observed, and the disposition of non-conforming products processed during the period of out-of-control operation. Records associated with non-conforming products shall be kept for a minimum of 3 years. Evidence of such compliance shall be verified by the qualifying activity of this specification as a prerequisite for qualification and continued qualification.

4.2 Classification of inspections. The inspections specified herein are classified as follows:

- a. Materials inspection (see 4.4).
- b. Final inspection (see 4.5).
- c. Qualification inspection (see 4.6).
- d. Quality conformance inspection (see 4.7).

4.3 Inspection conditions. Unless otherwise specified herein, all test inspection conditions shall be performed in accordance with the test conditions specified in the General Requirements of MIL-STD-202, as follows:

- a. Temperature: 25°C ±10°C.
- b. Relative humidity: 60 percent ±15 percent.
- c. Atmospheric pressure: 725 mm ±75 mm of mercury.

4.4 Materials inspection. Materials inspection shall consist of certification supported by verifying data that the materials listed in table II, used in fabricating the cables, are in accordance with the applicable referenced specifications or requirements prior to such fabrication.

TABLE II. Materials inspection.

Material	Requirement paragraph	Applicable documents
Ethylene tetrafluorethylene (ETFE)	3.5.6k	ASTM D-3159
Ethylene chlorotrifluoroethylene (E-CTFE)	3.5.6l	ASTM D-3275
Fiberglass	3.5.6d	MIL-Y-1140
Fluorinated ethylene propylene (FEP)	3.5.2.1t	L-P-389
Paint, aluminum	3.5.7b	TT-P-320
Polyethylene (PE)	3.5.2.1a	L-P-390
Polytetrafluoroethylene (PTFE)	3.5.6f	ASTM D-1457
Polyolefin, cross-linked	3.5.6o	
Rubber, butyl, insulating synthetic	3.5.2.1s	ASTM D-1352
Rubber, insulating synthetic	3.5.2.1x	ASTM D-470
Rubber, polychloroprene	3.5.6a,c,e,f	MIL-I-3930
Rubber, synthetic, semiconductor	3.5.2.1r	FED-STD-601
Tape, polyethylene-terephthalate	3.5.5c	MIL-I-631
Tubing, aluminum, seamless	3.5.3.2b	WW-T-700
Tubing, copper, seamless	3.5.3.2a	WW-T-799
Wire, aluminum-alloy (alclad 5056)	3.5.7a	ASTM B-211
Wire, aluminum, copper-clad	3.5.1.1g	ASTM B-566
Wire, copper, bare	3.5.1.1a	ASTM B-3
Wire, copper, beryllium (alloy 172)	3.5.1.1h	ASTM B-197
Wire, copper, silver-coated	3.5.1.1c,j	ASTM B-298
Wire, copper, tin-coated	3.5.1.1b	ASTM B-33
Wire, high resistance	3.5.1.1k	QQ-R-175
Wire, steel, copper-clad	3.5.1.1d	ASTM B-452
Wire, steel, copper-clad, silver-coated	3.5.1.1f	ASTM B-501
Wire, steel, galvanized	3.5.3.1.1	ASTM A-411
Rubber, polyurethane	3.5.6m	MIL-I-3930
Stranded inner conductors	3.5.1.2	ASTM B-8
Copper conductors for use in hook-up wire for electronic equipment	3.5.1.2	ASTM B-286

TABLE III. Final inspection.

Inspection		Requirement paragraph	Method paragraph
Semirigid cable <u>1/</u>	All other cable <u>2/</u>		
Continuity	Continuity	3.7.1	4.8.2
	Spark test	3.7.2	4.8.3
Voltage withstanding	Voltage withstanding	3.7.3	4.8.4
	Insulation resistance	3.7.4	4.8.5
	Out-of-roundness of jacket measurements	3.6.2	4.8.1.2

- 1/ Statistical sampling and inspection shall be in accordance with MIL-STD-105, general inspection level II. The acceptable quality level (AQL) shall be 1 percent for all the tests combined.
- 2/ Tests performed on each continuous length of cable.

4.5 Final inspection. Prior to the delivery of the cable, the tests in table III shall be performed, as applicable.

4.5.1 Failure.

- Semirigid cable - If the number of failures exceeds those allowed, the inspection lot shall be submitted to 100 percent inspection.
- All other cable - One or more failures shall be cause for refusal, except a spark test failure may be repaired or the cable length cut out.

4.6 Qualification inspection. Qualification inspection shall be performed at a laboratory acceptable to the Government (see 6.3) on sample units produced with equipment and procedures normally used in production. Group qualification shall be as specified in the appendix to this specification.

4.6.1 Sample. The sample of each cable type submitted for qualification inspection shall be of sufficient length to perform all the applicable tests in table IV.

TABLE IV. Qualification inspection.

Inspection	No. of specimens to be tested	Requirement paragraph	Method paragraph
<u>Group I</u>			
In-process inspection	Entire sample		4.5
Continuity	Entire sample	3.7.1	4.8.2
Spark test	Entire sample	3.7.2	4.8.3
Voltage withstanding	Entire sample	3.7.3	4.8.4
Insulation resistance <u>1/</u>	Entire sample	3.7.4	4.8.5
Visual and mechanical inspection	Entire sample	3.6	4.8.1
Physical dimensions	Entire sample	3.6	4.8.1
Marking	Entire sample	3.8	4.8.1
Workmanship	Entire sample	3.10	4.8.1

See footnotes at end of table.

TABLE IV. Qualification inspection - Continued.

Inspection	No. of specimens to be tested	Requirement paragraph	Method paragraph
<u>Group II</u>			
Corona extinction voltage <u>2/</u>	1	3.7.5	4.8.6
Characteristic impedance	1	3.7.6	4.8.7
RF transmission loss (attenuation) <u>2/</u>	2	3.7.7	4.8.8
Standing wave ratio (return loss) <u>2/</u>	2	3.7.8	4.8.9
Capacitance <u>2/</u>	1	3.7.9	4.8.10
Capacitance stability <u>2/</u>	1	3.7.10	4.8.11
Capacitance unbalance <u>3/</u>	1	3.7.11	4.8.12
Transmission unbalance <u>3/</u>	1	3.7.12	4.8.13
Mechanically induced noise voltage <u>4/</u>	1	3.7.13	4.8.14
Time delay <u>2/</u>	2	3.7.14	4.8.15
Aging stability <u>5/</u>	4	3.7.15	4.8.16
Stress-crack resistance <u>2/</u>	4	3.7.16	4.8.17
Outer conductor integrity <u>6/</u>	4	3.7.17	4.8.18
Cold bend <u>9/</u>	3	3.7.18	4.8.19
Dimensional stability <u>7/</u>	1	3.7.19	4.8.20
Contamination <u>8/</u>	1	3.7.20	4.8.21
Bendability <u>6/</u>	2	3.7.21	4.8.22
Flammability <u>2/</u>	1	3.7.22	4.8.23
Flame propagation <u>10/</u>	1	3.7.23	4.8.25
Acid gas generation <u>10/</u>	1	3.7.24	4.8.26
Halogen content <u>10/</u>	1	3.7.25	4.8.27
Immersion <u>10/</u>	1	3.7.26	4.8.28
Smoke index <u>10/</u>	1	3.7.27	4.8.29
Toxicity index <u>10/</u>	1	3.7.28	4.8.30
Durometer <u>10/</u>	1	3.7.29	4.8.31
Weathering <u>10/</u>	1	3.7.30	4.8.32
Abrasion resistance <u>10/</u>	5	3.7.31	4.8.33
Tear strength <u>10/</u>	6	3.7.32	4.8.34
Heat distortion <u>10/</u>	1	3.7.33	4.8.35
Physicals (aged) <u>10/</u>	1	3.7.34	4.8.36
Tensile strength and elongation <u>10/</u>	1	3.7.35	4.8.37
Weight	1	3.9	4.8.24

1/ Not applicable to solid types A and F dielectric cores.

2/ When specified.

3/ Applicable to two-conductor cables.

4/ Applicable to low noise cables.

5/ Not applicable to semirigid or cables with type IX jackets.

6/ Applicable to semirigid cables.

7/ Not applicable to time delay or braided inner conductor cables.

8/ Applicable to type IIa jackets.

9/ Not applicable to semirigid cables.

10/ Applicable to type XIV, polyolefin jacketed cables only.

4.6.2 Inspection routine. The samples shall be subjected to the inspections specified in table IV. The entire sample shall be subjected to the inspections of group I. The specimen length shall be cut from each sample as required, and subjected to inspections of group II.

4.6.3 Failure. One or more failures shall be cause for refusal to grant qualification approval.

4.6.4 Retention of qualification. To retain qualification, the contractor shall forward a report at 12-month intervals to the qualifying activity. The qualifying activity shall established the initial reporting date. The report shall consist of:

- a. A summary of the results of the tests performed for inspection of product for delivery (groups A and B), indicating as a minimum the number of lots that have passed and the number that have failed. The results of tests of all reworked lots shall be identified and accounted for.
- b. A summary of the results of tests performed for qualification verification inspection group C, including the number and mode of failures. The summary shall include results of all qualification verification inspection tests performed and completed during the 12-month period. If the summary of the test results indicates nonconformance with specification requirements, and corrective action acceptable to the qualifying activity has not been taken, action may be taken to remove the failing product from the qualified products list.

Failure to submit the report within 30 days after the end of each 12-month period may result in loss of qualification for the product. In addition to the periodic submission of inspection data, the contractor shall immediately notify the qualifying activity at any time during the 12-month period that the inspection data indicates failure of the qualified product to meet the requirements of this specification.

In the event that no production occurred during the reporting period, a report shall be submitted certifying that the company still has the capabilities and facilities necessary to produce the item. If during three consecutive reporting periods there has been no production, the manufacturer may be required, at the discretion of the qualifying activity, to submit representative cables of each type to testing in accordance with the qualification inspection requirements.

4.7 Quality conformance inspection.

4.7.1 Inspection of product for delivery. Inspection and final inspection in accordance with table III of product for delivery shall consist of groups A and B inspections.

4.7.1.1 Unit of product. A unit of product shall be 5,000 feet of cable of the same type designation. If a production run is less than 5,000 feet, then the quantity produced shall be one unit of product.

4.7.1.1.1 Inspection lot. The inspection lot shall consist of the number of units of product, offered for inspection at one time. All of the units of product in the inspection lot submitted shall have been produced during the same production period with the same materials and processes.

4.7.1.1.2 Sample unit. A sample unit shall be a unit of product selected at random from the inspection lot without regard to quality.

4.7.1.1.3 Sample unit size. Unless otherwise specified, the sample unit size shall consist of that number of sample units required by the inspection lot size, as determined by the sampling plans in MIL-STD-105.

4.7.1.1.4 Specimen. A specimen shall be an individual length of cable cut from the sample unit.

4.7.1.2 Group A inspection. Group A inspection shall consist of the inspections specified in table V.

4.7.1.2.1 Sampling plan. Statistical sampling and inspection shall be in accordance with MIL-STD-105 for general inspection level II. The acceptable quality level (AQL) shall be as specified in table V.

4.7.1.2.2 Rejected lots. If an inspection lot is rejected, the contractor may rework it to correct the defects, or screen out the defective units, and resubmit for reinspection. Resubmitted lots shall be inspected using tightened inspection and shall not thereafter be tendered for acceptance unless the former rejection or requirement of correction is disclosed. Such lots shall be separate from new lots, and shall be clearly identified as reinspected lots.

4.7.1.2.3 Disposition of sample units. Sample units from which a specimen has failed any of the group A inspection tests, shall not be delivered on any order, even though the inspection lot submitted is accepted.

TABLE V. Group A inspection.

Inspection	Requirement paragraph	Method paragraph	AQL (percent defective)
Visual and mechanical inspection	3.6	4.8.1	1
Physical dimensions	3.6	4.8.1	
Marking	3.8	4.8.1	
Workmanship	3.10	4.8.1	
Characteristic impedance	3.7.6	4.8.7	
RF transmission loss (attenuation)	3.7.7	4.8.8	
Standing wave ratio (return loss) <u>1/</u>	3.7.8	4.8.9	
Adhesion of conductors	3.6.4	4.8.1.4	1
Eccentricity of inner conductor	3.6.3	4.8.1.3	1

1/ As applicable.

4.7.1.3 Group B inspection. Group B inspection shall consist of the inspections specified in table VI.

4.7.1.3.1 Sampling plan. The sampling plan shall be in accordance with MIL-STD-105 for special inspection level S-3. The sample size shall be based on the inspection lot size from which the sample was selected for group A inspection. The AQL shall be as shown in table VI.

4.7.1.3.2 Rejected lots. If an inspection lot is rejected, the contractor may rework it to correct the defects, or screen out the defective units, and resubmit for reinspection. Resubmitted lots shall be inspected using tightened inspection and shall not thereafter be tendered for acceptance unless the former rejection or requirement of correction is disclosed. Such lots shall be separate from new lots, and shall be clearly identified as reinspected lots.

TABLE VI. Group B inspection.

Inspection	Requirement paragraph	Method paragraph	AQL (percent defective)
Corona extinction voltage <u>1/</u>	3.7.5	4.8.6	4
Capacitance	3.7.9	4.8.10	
Capacitance unbalance <u>1/</u>	3.7.11	4.8.12	
Transmission unbalance <u>1/</u>	3.7.12	4.8.13	
Mechanically induced noise voltage <u>1/</u>	3.7.13	4.8.14	
Time delay <u>1/</u>	3.7.14	4.8.15	
Cold bend <u>2/</u>	3.7.18	4.8.19	
Weight	3.9	4.8.24	
Tear strength <u>1</u>	3.7.32	4.8.34	4

1/ As applicable.

2/ Not applicable to semirigid cables.

4.7.1.3.3 Disposition of sample units. Sample units from which a specimen has failed any of the group B inspection tests shall not be delivered on any order, even though the inspection lot submitted is accepted.

4.7.2 Group C inspection. Group C inspection shall consist of the inspections specified in table VII. Group C inspection shall be made on sample units selected from inspection lots which have passed the groups A and B inspection.

4.7.2.1 Sampling plan. Sample units shall be selected from those types covered by a single specification sheet in accordance with table VIII, 3 months after the date of notification of qualification, except when the total production in a 3-month period is less than two units of product (10,000 feet) inspection need not be made until either production is at least 2 units of product or a total of 6 months has elapsed since the inspection was performed in which case only one sample unit shall be tested.

TABLE VII. Group C inspection.

Inspection	Requirement paragraph	Method paragraph
Capacitance stability <u>1/</u>	3.7.10	4.8.11
Aging stability <u>1/</u>	3.7.15	4.8.16
Stress-crack resistance <u>1/</u>	3.7.16	4.8.17
Outer conductor integrity <u>1/</u>	3.7.17	4.8.18
Dimensional stability <u>1/</u>	3.7.19	4.8.20
Contamination <u>2/</u>	3.7.20	4.8.21
Bendability <u>1/</u>	3.7.21	4.8.22
Flammability <u>1/</u>	3.7.22	4.8.23
Heat distortion <u>1/</u>	3.7.33	4.8.35
Tensile strength and elongation <u>1/</u>	3.7.35	4.8.37
Physicals (aged) <u>1/</u>	3.7.34	4.8.36

1/ When specified.

2/ Applicable to type IIa jackets.

TABLE VIII. Sampling plan for group C inspection.

Units of product from 3-month's production	Sample unit size
2	1
3 to 8, inclusive	2
9 to 30, inclusive	3
31 to 80, inclusive	4
81 to 130, inclusive	5
131 to 180, inclusive	6
181 to 240, inclusive	7
241 to 300, inclusive	8

4.7.2.1.1 Failures. If one or more specimens fail to pass group C inspection, the inspection lot shall be considered to have failed.

4.7.2.1.2 Disposition of specimens. Specimens that have been tested to group C inspection shall not be delivered on the contract or purchase order.

4.7.2.1.3 Noncompliance. If a sample fails to pass group C inspection, the manufacturer shall notify the qualifying activity and the cognizant inspection activity of such failure and take corrective action on the materials or processes, or both, as warranted, and on all units of product which can be corrected and which are manufactured under essentially the same materials and processes, and which are considered subject to the same failure. Acceptance and shipment of the product shall be discontinued until corrective action, acceptable to the qualifying activity has been taken. After the corrective action has been taken group C inspection shall be repeated on additional sample units (all tests and examinations, or the test which the original sample failed, at the option of the qualifying activity). Groups A and B inspections may be reinstituted; however, final acceptance and shipment shall be withheld until the group C inspection has shown that the corrective action was successful. In the event of failure after reinspection, information concerning the failure shall be furnished to the cognizant inspection activity and the qualifying activity.

4.7.3 Inspection of packaging. The sampling and inspection of the preservation, packing and container marking shall be in accordance with the requirements of MIL-C-12000.

4.8 Methods of inspection. Test parameters given in the following tests are not to be assumed as the cable operating conditions, temperatures or limits. Methods of inspection given in the specification shall be the only acceptable methods unless an alternate method has been agreed to by the qualifying authority prior to the performance of the test. The test methods described herein are the preferred methods and shall be the referee method in cases of dispute.

4.8.1 Visual and mechanical examination (see 3.6). The cable shall be examined to verify that the design, construction, physical characteristics and dimensions, marking, and workmanship are in accordance with the applicable requirements (see 3.6, 3.8, and 3.10).

4.8.1.1 Diameter measurements (see 3.6.1).

- a. All components, except the dielectric core of semirigid cables. Measurements shall be made on a suitable length (12 inch minimum) of cable taken from the end of the sample unit. Inner components shall be made accessible by stripping and removing the outer components carefully so as not to nick, cut, cold-work, or otherwise, damage the component to be measured. Four points for measurement shall be located 3 to 4 inches apart along the specimen length. Measurements shall be made at each point in two mutually perpendicular planes, so that a total of eight measurements are performed on each specimen. Measurements shall be made with a micrometer caliper or any other instrument of equal accuracy.
- b. Dielectric core of semirigid cables. The outer diameter of the dielectric core shall be determined by measuring the inner diameter of the solid outer conductor. Measurements shall be made on four specimens, each 0.5 inch approximately in length, taken from the end of the sample unit. The specimens shall be cut squarely and carefully deburred. Measurements shall be made by means of plug gauges, or an adjustable plug hole gauge and a micrometer, or any other instrument of equal accuracy.

4.8.1.2 Out-of-roundness of jacket measurements (see 3.6.2). When specified (see 3.1), the out-of-roundness of the jacket shall be monitored on a continuous production basis, and the jacket diameter shall be as specified (see 3.1). The out-of-roundness measurements shall be permanently recorded with a device capable of producing continuous graphic records. Two recordings shall be made, as nearly simultaneously as possible, of the outside diameter 90° apart and a point in the manufacturing process where further dimensional change will not occur. The recordings shall be permanent and reproducible by a common commercial process. The technique used (including the detector, recorder and associated components) shall have a response capable of recording changes in the diameter with a sensitivity of 0.001 inch along the length of cable at whatever speed the cable is traveling. The strip chart response time shall be compatible with the remainder of the system. The pen traverse shall be large enough to distinguish changes of diameter of 0.001 inch. The chart speed relative to the cable speed shall be such that the recording must be identifiable to within 2 feet of the point on the cable length measured. Each foot of cable shall be represented by no less than 0.05 inch of recording paper.

4.8.1.3 Eccentricity of inner conductor (see 3.6.3).

4.8.1.3.1 Procedure. Four specimens, each 1 inch approximately in length, shall be cut from the end of the sample unit. The outer components of the cable shall be removed down to the dielectric core. The ends of the specimen shall be cut squarely and carefully deburred. The eccentricity, in terms of displacement of length, shall be measured with a machinist's microscope, or a comparator, or any other instrument capable of yielding a resolution of at least .0001 inch. At spacings approximately 45° apart around the periphery of the inner conductor, measurements shall be taken of the dielectric wall thickness. The thickest measurement (T_{max}) and the thinnest measurement (T_{min}) shall then be used to compute the displacement, using the following formula:

$$\% \text{ Eccentricity} = \frac{T_{max} - T_{min}}{\text{Measured diameter of core}} \times 100$$

The percent eccentricity of the inner conductor shall be within the specified requirements (see 3.1).

4.8.1.3.2 Alternate method. As an alternate method of measurement that is more applicable for determining the eccentricity of the inner conductor of a semirigid cable, lay the sample in a Vee-shaped trough to which a dial indicator has been rigidly fastened in such a manner as to preclude movement of the indicator with respect to the trough, and to allow a reading of the inner conductor position with respect to the outer surface of the cable. Four specimens each approximately 6.0 inches long, shall be cut from the end of the sample unit. Prepare the specimen by exposing approximately .250 inch of the inner conductor at one end of each specimen. The dial indicator shall be capable of yielding a resolution of at least .0001 inch. The specimen shall be slowly rotated in the trough and the difference in dial indicator readings shall be noted through a rotation of 360°. Care shall be taken to avoid bending the inner conductor during the rotation operation. The difference in the dial indicator reading is the total indicator reading (TIR), from which the % eccentricity may be computed using the following formula:

$$\% \text{ Eccentricity} = \frac{\text{Difference in dial indicator readings}}{\text{Measured diameter of core}} \times 100$$

4.8.1.4 Adhesion of conductors (see 3.6.4).

4.8.1.4.1 Specimen.

- a. Two specimens of each cable shall be cut from the end of the sample unit. Each specimen shall be prepared as shown on figures 1 and 2. Stripping shall be done carefully. For semirigid cables, no more than .250 inch of material shall be removed at one time.

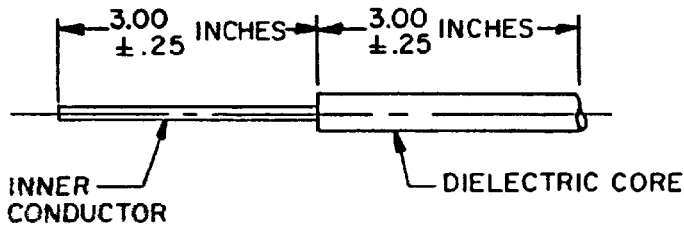


FIGURE 1. Stripping dimensions for flexible cables.

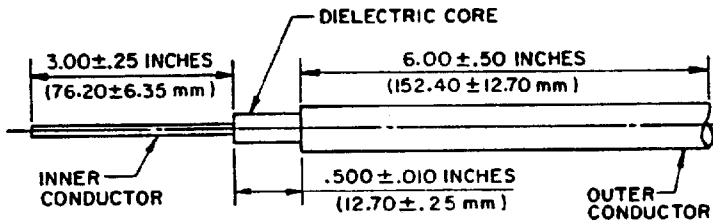


FIGURE 2. Stripping dimensions for semi-rigid cables.

- b. The adhesion to conductors test shall be performed with a tensile tester and a test fixture such as shown on figures 3 and 4. The diameter of the hole in the test plate shall be $.004 \pm .001$ inch larger than the diameter of the applicable inner conductor or dielectric core. The inner conductor or dielectric core extending through the test plate hole shall be pulled with a constantly increasing force at a rate not to exceed 0.5 inch per minute. Avoid sudden pulls and jerking. Conductor adhesion shall be defined as the highest tensile tester reading obtained when the conductor-to-core bond is broken. In performing this test, physical handling of the specimen shall be kept to a minimum to avoid specimen degradation. The adhesion to conductor requirement, as noted by the reading on the tensile tester shall meet the specified value (see 3.1).

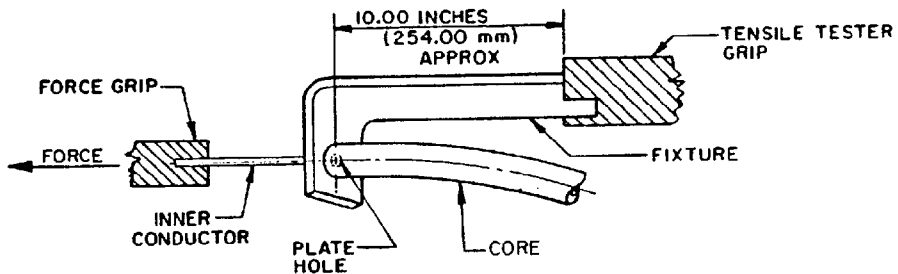


FIGURE 3. Typical test fixture for use with flexible cables.

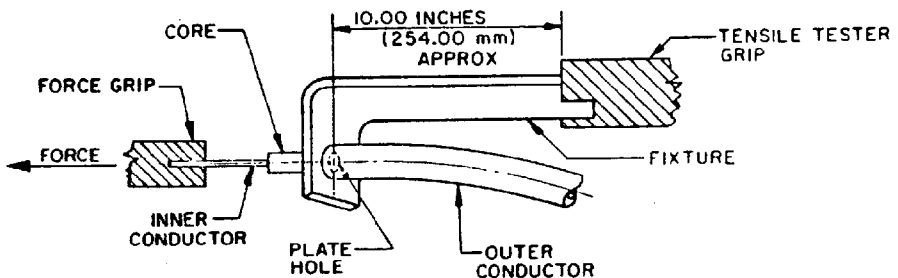


FIGURE 4. Typical test fixture for use with Semi-rigid cables.

- c. When semirigid cables are tested in accordance with the preceding procedure and the conductor-to-core bond is not broken at the specified maximum force (see 3.1), the test shall be repeated with additional specimens and the following modifications:

- (1) The length of the outer conductor section (see figure 2), shall be 1.00 inch $\pm$.12 inch (25.4 $\pm$ 3.05 mm), in lieu of 6.00 $\pm$.50 inches (152.40 $\pm$ 12.70 mm).
- (2) The force grip (see figure 4) shall be applied to the core in lieu of the inner conductor.
- (3) Conductor adhesion shall not exceed the specified maximum value (see 3.1).

4.8.2 Continuity (see 3.7.1). To establish continuity, 25 volts dc maximum shall be applied to both ends of each conductor and shield of the cable through an appropriate indicator, such as an ohmmeter light, or buzzer. The test voltage may be applied to the conductors and shields individually or in series.

4.8.3 Spark test (see 3.7.2). The specimen shall be tested for jacket spark in accordance with method 6211 of FED-STD-228. A test voltage (see 3.1) at a frequency between 48 and 62 Hz or 3.0 $\pm$.5 kHz shall be applied between the outermost braid or shield and the outer surface of the jacket. Either the 60 Hz or the 3 kHz is acceptable. In the event of conflict, the 3 KHz test will be the governing test.

4.8.4 Voltage withstanding (see 3.7.3). The specimen shall be tested in accordance with method 6111 in accordance with FED-STD-228, except that the specimen shall not be immersed in water but tested dry. The specified test voltage (see 3.1) at a frequency of 60 Hz shall be applied to all samples for a minimum of 1 minute. The following details shall apply:

- a. For coaxial cables. The test voltage shall be applied between the inner and the outer conductor, with the outer conductor grounded.
- b. For triaxial cables. In addition to (a) above, 500 V dc shall be applied between the outer conductor and the extra shield with the extra shield grounded.
- c. For two-conductor cables. The test voltage shall be applied between the two inner conductors. In addition, the test voltage shall be applied individually between each inner conductor and the outer conductor with the outer conductor grounded.

4.8.5 Insulation resistance (see 3.7.4). The specimen shall be measured with an apparatus suitable to verify compliance with the applicable detail specification requirement. The following details shall apply:

- a. Unless otherwise specified (see 3.1), the measurement error, including the error of the test voltage source, the error of the indicating circuit, and the error in measurement of the mechanical specimen lengths, shall not exceed $\pm$ 15 percent.
- b. The voltage (see 3.1) shall be 200 volts dc minimum and the polarity shall be such that the outer conductor is at ground potential.
- c. Measurements shall be made between the conductors specified (see 3.1).

- d. Unless otherwise specified (see 3.1), readings shall be taken immediately after an uninterrupted 2-minute electrification period. However, a stable, or an increasing reading indicating compliance with the specification requirement obtained before elapse of the 2-minute electrification period shall be acceptable.
- e. The insulation resistance of the test specimen shall be calculated from the formula

$$R = \frac{M \times L}{1000}$$

Where R = Insulation resistance for 1000 feet in megohms.

M = Indicator reading in megohms.

L = Test specimen length in feet, measured between outer conductor ends.

4.8.6 Corona extinction voltage (see 3.7.5). The cable test specimen shall be subjected to a gradually increasing sinusoidal voltage until a detector indicates a sustained corona discharge. The following details shall apply:

- a. The sensitivity of the detection equipment shall permit observation of corona of five picocoulombs or less.
- b. The cable specimen shall be from 2 to 5 feet in length. The ends of the cable shall be made corona free. A suggested method for making the ends corona free is shown on figure 15 (see 6.7).
- c. After the cable preparation, connect the cable test specimen to a voltage source. Both ends may be immersed in insulating oil to prevent corona discharge at the ends.
- d. The test voltage shall be applied at room ambient conditions. The frequency of the test voltage shall be between 48 and 62 Hz.
- e. Slowly increase the 48 to 62 Hz test voltage until the detector indicates a sustained corona discharge or reaches two times the specified corona extinction voltage.
- f. If sustained corona discharge is indicated, the voltage shall then be decreased slowly until the corona extinction point is observed. The corona extinction voltage is defined as the voltage at which sustained discharge ceases. If sustained corona has not been observed at two times the specified corona extinction level the requirement is considered to have been satisfied.
- g. When specified (see 3.1), the corona extinction voltage test shall be performed at the specified altitude equivalent reduced pressure.

4.8.7 Characteristic impedance (see 3.7.6).

4.8.7.1 Specimen. The specimen shall be 10 feet minimum or 2 dB maximum at 3 GHz whichever is the shorter.

4.8.7.2 Procedure. The specimen shall be prepared for testing by assembling appropriate connections to the cable ends. The equipment shall include a Time Domain Reflectometer (TDR). The rise time of the TDR shall be 150 picoseconds or less, and the vertical sensitivity of the system shall provide for a minimum resolution of one major scale division. A precision air-line of the same nominal characteristic impedance as the specimen shall be connected between the TDR and the connector-cable assembly. The characteristic impedance of the specimen shall then be measured compared to the precision air-line. The connector-cable assembly shall then be turned end-to-end and the measurement repeated. For cables of other than 50 and 75 ohms characteristic impedance, where precision air-lines, loads, or proper impedance measuring equipment are not available, the characteristic impedance may be determined by calculation from the capacitance measurement determined (see 4.8.10) and the velocity of propagation measurement determined, using the following formula:

$$Z_0 = \frac{101,670}{\text{Velocity of propagation (\%)} \times \text{Capacitance (pF/ft)}}$$

4.8.8 RF transmission loss (attenuation) (see 3.7.7). The RF transmission loss (attenuation) shall be determined in accordance with the following procedures or an alternate method acceptable to the Government. In the event of dispute the method outlined herein shall be used (see figure 5).

4.8.8.1 Specimen. The cable specimen for swept frequency testing shall be of sufficient length to exhibit no less than 1 dB loss at the low end of the frequency range. The maximum length shall be such that the specimen exhibits a loss at the highest swept frequency no greater than the dynamic range of the calibrated measurement system less 10 dB. If the measured loss of a specimen at the highest frequency exceeds that value, an additional specimen of shorter length shall be used. The specimen for fixed frequency testing shall be long enough to exhibit a loss no less than 3 dB and no greater than the dynamic range of the measurement system less 10 dB. Both ends of the specimen shall be terminated by suitable connectors having interfaces in accordance with MIL-STD-348.

4.8.8.2 Procedure. When required a swept frequency RF transmission loss technique shall be used to determine the attenuation within the specified frequency range (see 3.1). Figure 5 shows a block diagram of typical equipment to be used for the measurements. Steps 1 through 3 apply to the coaxial cable. The test setup shall include a display of RF transmission loss in dB as a function of frequency. For qualification testing recordings of the display are required for each step. A curve representing the specification limit shall be shown in the Step 3 chart to permit a direct comparison with the transmission loss of the test specimen. The zero dB reference level is established with matching pads 1 and 2 connected directly to each other in step 1. System amplitude accuracy is verified in step 2 by measuring the RF transmission loss of calibrated attenuators over the specified frequency range (see 3.1). The calibrated attenuators shall have nominal values covering the anticipated measurement loss values. Their calibration data shall be accurate within the following limits:

<u>Nominal value, dB</u>	<u>Uncertainty, dB</u>
Up to 10	±.1
Over 10 to 20	±.2
Over 20 to 30	±.3
Over 30 to 40	±.4
Over 40 to 50	±.5

System amplitude accuracy shall be 5% or better over the specified frequency range (see 3.1). When tests at fixed frequencies are specified, a tunable or fixed frequency source may be substituted for the swept RF source and the X-Y display may be omitted. For tests on specimens having a characteristic impedance widely different from that of the measurement system, suitable impedance matching devices may be used in combination with the pads. The pads may consist of suitable lengths of cable similar to that being tested. For tests on twin conductor (balanced) cables, appropriate baluns (balanced-to-unbalanced transformers) are added to the system as shown in steps 4 and 5. Attenuation at any frequency is expressed by the following formula:

$$\text{Attenuation, dB/100 feet} = \frac{\text{Measured loss, dB} \times 100}{\text{Specimen length, feet}}$$

4.8.9 Standing wave ratio (return loss) (see 3.7.8). The standing wave ratio (return loss) shall be measured in accordance with one of the following procedures or another method acceptable to the Government. In the event of dispute the slotted line method outlined herein shall be used for frequencies above 2 GHz; for frequencies up to 2 GHz either the slotted line or the RF bridge may be used.

4.8.9.1 Swept frequency slotted line system. Diagrams for the swept frequency slotted line system check out and measurement procedures are shown on figure 6. In the basic measurement setup of figure 6 detector 1 provides a feedback signal to the swept RF source in order to normalize the output signal of detector 2. The frequency-amplitude characteristics of detectors 1 and 2 should be matched within 0.5 dB. The slotted line shall have a precision hermaphroditic output connector and its residual VSWR shall be less than $1.006 + .003 F$ (F in GHz). To measure standing wave ratio (return loss) several sweeps are made with the slotted line probe incrementally positioned over at least a half wave length at the lowest frequency of interest. In this manner an X-Y display is generated whose upper and lower envelope limits represent maximum and minimum amplitudes of the standing wave for each frequency in the test band. A base line may be generated by making a sweep with no input to the measurement channel amplifier. The resultant X-Y display is calibrated according to the characteristics of the measurement channel detector and amplifier, e.g., linear, square law, logarithmic, etc. The standing wave ratio test system is checked out by successively terminating the slotted line with the elements shown in steps 1 and 2 and sweeping the frequency over the specified test band (see 3.1). In step 1 the system standing wave ratio shall be less than $1.02 + .004 F$ (F measured in GHz). In step 2 the system SWR shall be as specified (see 3.1). For qualification the measurement is made as in step 3 or 4. The minimum cable length shall be as specified (see 3.1). Group A tests may be performed as in step 5.

4.8.9.2 Swept radio frequency bridge system. Diagrams for the swept RF bridge system check out and measurement procedures are shown on figure 7. The 0 dB reference for bridge directivity (up to 2 GHz) is the average of the precision open and short signals of step 1. Effective directivity of the system determined by steps 3 and 6 shall be 10 dB greater than the specified cable return loss (see 3.1). The 0 dB reference for steps 8 or 9 is a short at the standard test connector interface. The minimum cable length for step 8 shall be as specified (see 3.1). Step 8 is to be used for qualification. Step 9 may be used for group A testing. The standard precision adapter interface shall conform to IEEE Standard 287. Standard precision adapters shall not exceed the specified VSWR requirements (see 3.1). Standard test adapter designs shall be approved by the military qualifying agency.


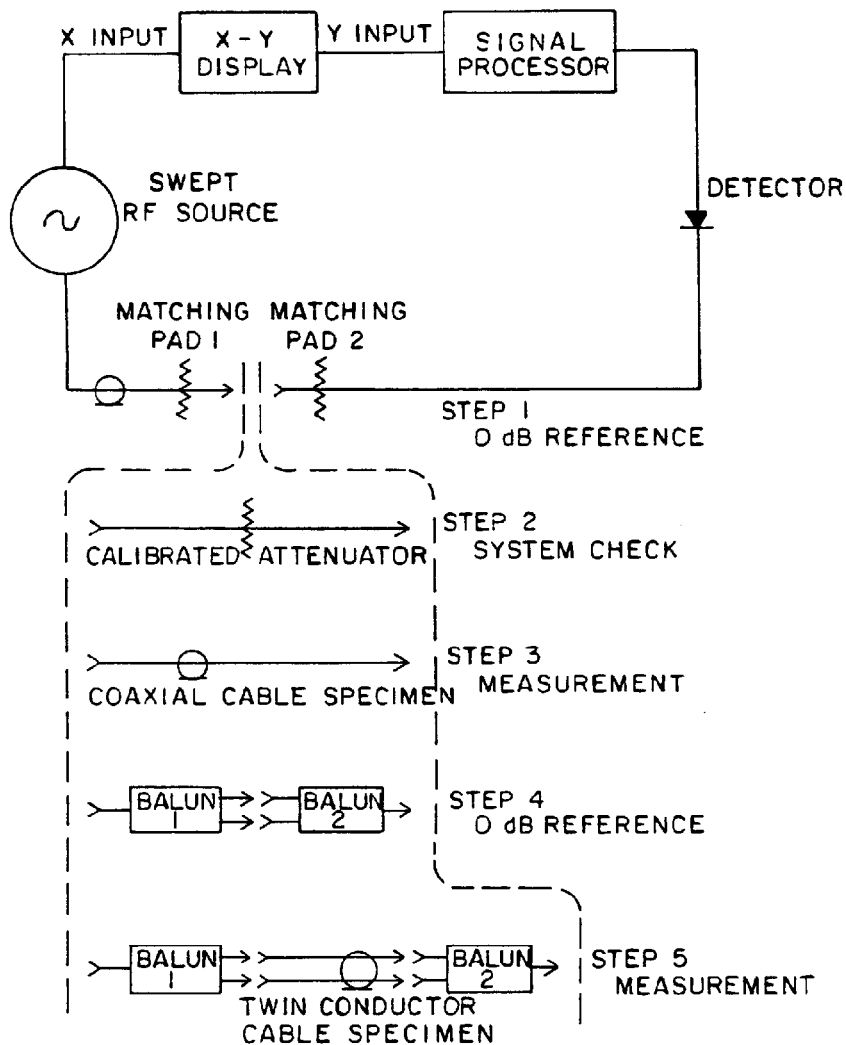


FIGURE 5. RF transmission loss (attenuation).

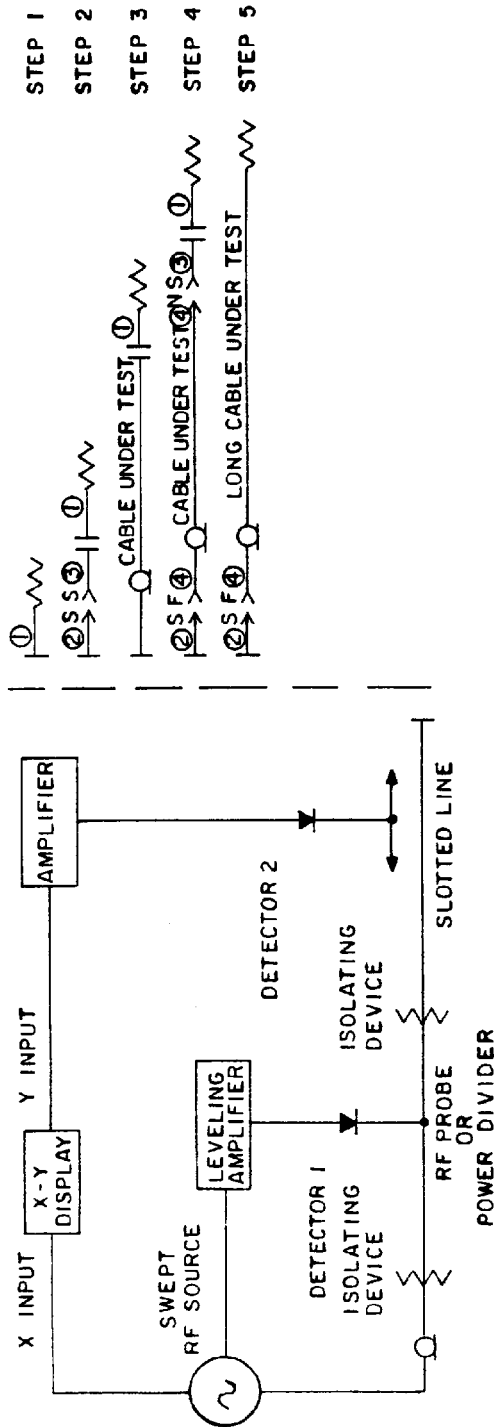


NOTES:

1. Precision termination.
2. Standard precision adapter, maximum VSWR as specified, (see MIL-C-39012, 3.1).
3. Standard precision adapter, maximum VSWR as specified, (see MIL-C-39012, 3.1)
4. Selected MIL-C-39012 connectors

- Precision hermaphroditic connectors (see IEEE 287)
- Standard test connector interfaces (see MIL-STD-348)
- MIL-C-39012 connector interfaces (see MIL-STD-348)

FIGURE 6. Swept frequency slotted line method for standing wave ratio (return loss) test.

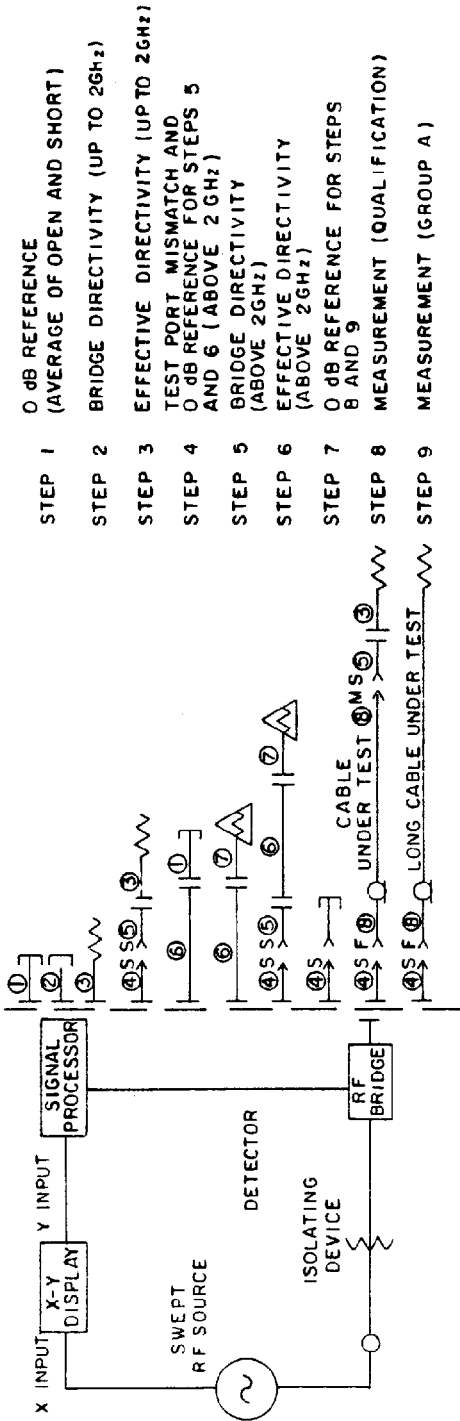

—|— Precision hermetic connectors (see IEEE 287)
 S S Standard test connector interfaces (see MIL-STD-348)
 M F MIL-C-39012 connector interfaces (see MIL-STD-348)

—|— short
 —|— open

NOTES:

1. Precision short
2. Precision open.
3. Precision termination.
4. Standard precision adapter, maximum VSWR as specified (see MIL-C-39012, 3.1)
5. Standard precision adapter, maximum VSWR as specified (see MIL-C-39012, 3.1).
6. Precision airline, maximum VSWR 1.006 + .002F (F in GHz).
7. 20 dB offset
8. Selected MIL-C-39012 connector.

FIGURE 7. Swept frequency RF bridge method for standing wave ratio (return loss) test.

4.8.10 Capacitance (see 3.7.9). The capacitance, in picofarads per foot, of the specimen shall be measured at 1 kHz, unless otherwise specified (see 3.1). The following details shall apply:

- a. The specimen length shall be less than 1/40 wavelength but not less than 5 feet.
- b. Coaxial cables. The capacitance shall be measured between the inner conductor and the outer conductor, with the outer conductor grounded.
- c. Two-conductor cables. The capacitance between the two inner conductors shall be measured by a two or three terminal technique.
 - (1) Two-terminal method. With the outer conductor connected to the ground terminal of the capacitance bridge, the capacitance shall be determined from the following formula:

$$\text{Capacitance} = \frac{2 (C_a + C_b) - C_c}{4}$$

Where: C_a = Capacitance between no. 1 conductor and no. 2 conductor, with no. 2 conductor connected to the outer conductor.

C_b = Capacitance between no. 2 conductor and no. 1 conductor, with no. 1 conductor connected to the outer conductor.

C_c = Capacitance between no. 1 and no. 2 conductors (when tied together) and the outer conductor.

- (2) Three-terminal method. The capacitance shall be determined from the following formula:

$$\text{Capacitance} = C_d + \frac{C_e + C_f}{4}$$

Where: C_d = Capacitance between no. 1 conductor and no. 2 conductor, with the outer conductor connected to the ground terminal of the capacitance bridge.

C_e = Capacitance between no. 1 conductor and the outer conductor, with no. 2 conductor connected to ground.

C_f = Capacitance between no. 2 conductor and the outer conductor, with no. 1 conductor connected to ground.

4.8.11 Capacitance stability (see 3.7.10). The capacitance, in picofarads per foot, shall be measured as specified in 4.8.10. The length of the specimen shall be approximately 50 feet, except that for cables with solid outer conductors the length of the specimen shall be approximately 10 feet. The specimen shall be subjected to the applicable temperature cycle shown in table IX, for a total of three cycles. Test temperatures for cables with dielectric cores not listed in table IX shall be as specified (see 3.1). Capacitance measurements shall be made initially and after each step.

TABLE IX. Temperature cycling.

Step	Type A dielectric C temperature	Type F dielectric C temperature	Time hours
1	+75 ±2	+250 ±5	4 to 8
2	+25 +10, -5	+25 +10, -5	4 minimum
3	-40 ±2	-55 ±2	4 to 8
4	+25 +10, -5	+25 +10, -5	4 minimum

4.8.12 Capacitance unbalance (see 3.7.11). The capacitance, in picofarads per foot, shall be measured as specified in 4.8.10. The length of the specimen shall be as specified in 4.8.10. The capacitance between the two inner conductors of the two-conductor cable shall be measured by the two- or three-terminal technique as specified in 4.8.10. The capacitance unbalance in percent shall be determined from the following formula:

a. Two-terminal method:

$$\text{Capacitance unbalance} = \frac{400 (C_a - C_b)}{2 (C_a + C_b) - C_c}$$

b. Three-terminal method:

$$\text{Capacitance unbalance} = \frac{400 (C_e - C_f)}{4 C_d + C_e - C_f}$$

4.8.13 Transmission unbalance (see 3.7.12). The transmission unbalance of a two-conductor coaxial cable is defined as the ratio of the absolute magnitude of the vector difference of the voltages across each half of a terminating resistor to one half of the absolute magnitude of the vector sum of the two voltages, expressed mathematically as follows:

$$\text{Transmission unbalance (TUB)} = \frac{|V_2 - V_1|}{1/2 |V_2 + V_1|} \times 100\%$$

Where: TUB = Transmission unbalance, in percent.

V_2 = Vector voltage across half of the terminating resistor, in volts.

V_1 = Vector voltage across the other half of the terminating resistor, in volts.

4.8.13.1 Specimen. The specimen to be measured shall be approximately 100 feet in length.

4.8.13.2 Equipment. The accuracy of the measuring equipment shall be ±2 percent over the test frequency (see 3.1). Figure 8 shows a block diagram of the transmission unbalance test equipment.

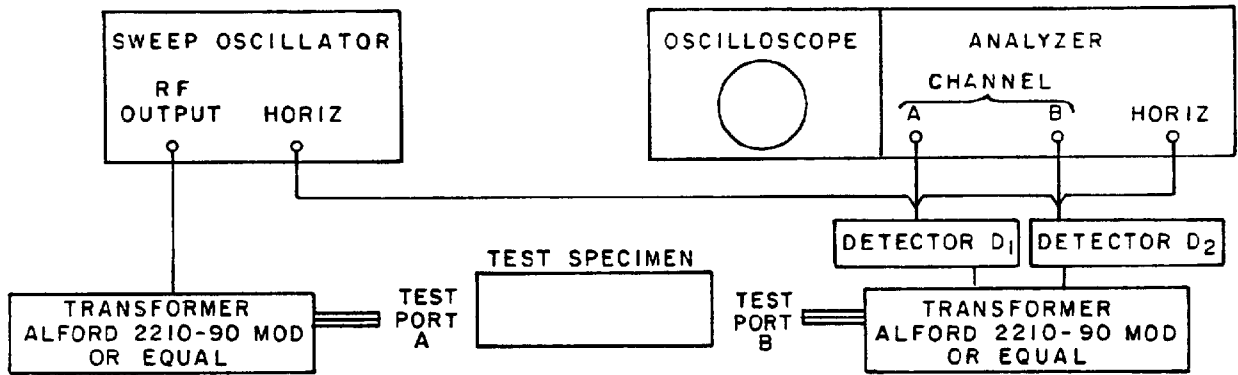


FIGURE 8. Block diagram of transmission unbalance test equipment.

4.8.13.3 Measurement. The input transformer transmits two signals which are vectorially equal down the two-conductor line. The signal from detector no. 1 on the output transformer is the magnitude of the vector difference of the voltages across each half of the terminating resistor, and the signal from detector no. 2 is the magnitude of the vector sum of the two voltages. The oscilloscope has logarithmic vertical amplifiers that allow the measurement of the ratio of the signals from the two detectors, expressed in decibels as follows:

$$TUB(\%) = 200 / \left[\text{ANTILOG}_{10} \left(\frac{\text{dB scope}}{20} \right) \right]$$

The residual error of the tests system may be obtained by removing the sample, connecting the respective test ports and measuring the system unbalance. The maximum unbalance of the specimen shall not exceed the specified value (see 3.1).

4.8.13.4 Calibration of transmission unbalance system. Calibration shall be performed as follows:

- a. Connect test port A to test port B.
- b. Switch on the frequency markers of the sweep oscillator. Connect channel A of detector no. 2 to the generator video input, and the generator vertical to the scope channel A port. By varying the frequency dial and sweep width controls of the sweep oscillator, obtain the required test frequency range.
- c. Remove detector no. 1 from detector port P and replace it with a 50-ohm load. Connect channel A to detector no. 2 of the scope.
- d. Obtain a signal from detector no. 2 on channel A. Trace this signal on the scope screen. Preset channel A attenuator to zero.
- e. Insert a 10-dB pad between detector port no. 2 and detector no. 2.
- f. Adjust channel A attenuator so that the average of the scope display and traced line are equal.
- g. Insert a 20-dB pad between detector port no. 2 and detector no. 2. Draw the trace on the face of the scope.
- h. Remove detector no. 2 from detector port no. 2, and replace it with detector no. 1. Connect the lead from detector to channel B vertical input.
- i. Obtain trace from detector no. 1 by inserting a 20-dB pad between detector and connecting port. The frequency tracking of the two detector should not vary more than ± 0.5 dB.
- j. Repeat Steps (d), (e) and (f), with detector no. 1 connected to detector port no. 2. The lead from detector no. 1 must be connected to the channel B vertical input of the scope.
- k. Return detectors to their original positions.

4.8.13.5 Measurement procedure for transmission unbalance system. Measurements shall be performed as follows:

- a. Prepare specimen and install applicable connectors.
- b. Connect specimen between test port A and test port B.

- c. Preset variable attenuators A and B to zero.
- d. Switch the display control of the scope to channel A and B position.
- e. Using the channel A variable attenuator, position the channel A trace at the center of the scope screen.
- f. Using the channel B variable attenuator, position the channel B trace so that it covers the channel A trace.
- g. The difference, in dB, of the channel A and B variable attenuators is the unbalance of the two signals.
- h. Convert the dB difference of channel A and B to the percentage of transmission unbalance by using table X.

TABLE X. Relationship between transmission unbalance and the difference in signals.

Transmission unbalance	Difference in signal	Transmission unbalance	Difference in signal	Transmission unbalance	Difference in signal
<u>percent</u>	<u>dB</u>	<u>percent</u>	<u>dB</u>	<u>percent</u>	<u>dB</u>
2	40.0	12	24.5	22	19.0
3	36.0	13	24.0	23	18.9
4	34.0	14	23.0	24	18.4
5	32.0	15	22.5	25	18.0
6	30.0	16	22.0	26	17.8
7	29.0	17	21.5	27	17.4
8	28.0	18	21.0	28	17.0
9	27.0	19	20.5	29	16.8
10	26.0	20	20.0	30	16.4
11	25.6	21	19.5		

4.8.14 Mechanically induced noise (see 3.7.13). The electrical noise generated in a cable by mechanical motion shall be determined by the following test.

4.8.14.1 Preparation of cable. Cut cables to be tested into 7-foot lengths. Fit one end of cable with a suitable connector. Remove 2 inches of the outer jacket from the other end of the cable leaving the braid intact. Push braid back and cut off 1 inch of the dielectric and center conductor. Cover the open end with three layers of electrical tape. Pull braid over the tape. Twist and solder to form an interference shield.

4.8.14.2 Instrumentation.

a. Amplifier.

- (1) Input impedance - 10 megohms minimum.
- (2) Frequency response - dc to 1 megahertz minimum.
- (3) Sensitivity - 10 microvolts/centimeter minimum.

b. Oscilloscope.

c. Recorder.

(1) For digital, storage scope with X-Y output to X-Y recorder.


(2) For nondigital, storage scope oscilloscope camera.

d. Appropriate weight with cable clamp. One pound weight for cables up to 0.2 inch in diameter and a five-pound weight for cable over 0.2 inch in diameter.

e. Six cable clamps of suitable size and circumferential compression type.

f. Suitable cable connector for interfacing with amplifier.

4.8.14.3 Equipment set-up (see figure 9). Clamp the cable in place so that the interference shield is just beyond three of the clamps and the inside clamps are 4 feet apart and such that 5 feet of slacked cable hangs freely between the support. Clamp the weight midspan of cable (that is, 30 inches from either end of the 5 feet of cable supported between the clamps). Connect the cable to be tested to the amplifier and oscilloscope. Shield as necessary to prevent noise pick-up.

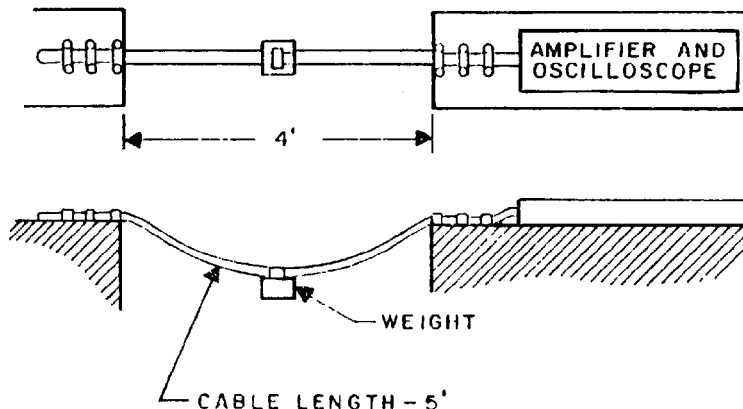FIGURE 9. Equipment setup.

4.8.14.4 Calibration of instruments. Set the gain of the amplifier so the specified maximum peak-to-peak noise can be easily determined. Calibrate the amplifier and oscilloscope for an accuracy of ± 5 percent. Set the oscilloscope in the single sweep mode with a sweep speed of 1 cm per second and the sensitivity to 10 $\mu\text{V}/\text{cm}$, lower frequency 3 dB response to .1 Hz, upper frequency 3 dB response to 10 kHz.

4.8.14.5 Test procedure. Pull cable through 90° arc until cable, weight, and clamp are in a horizontal plane. If a camera is used, open the camera shutter, trigger the sweep, and release the weight. A mechanical release device may be used, if desired to assure repeatability of the measurements. Repeat this procedure until eight individual sweeps have been recorded.

4.8.15 Time delay (see 3.7.14).

4.8.15.1 Specimen. Two specimens shall be tested for time delay. The test frequency shall be as specified (see 3.1). The length of the specimen shall be determined from the following formula:

$$L = \frac{983.6}{f \sqrt{e}}$$

Where: L = Specimen length, in feet.

f = Specified frequency, in MHz.

e = Dielectric constant of cable dielectric core.

4.8.15.2 Procedure. The time delay measurement shall be performed as follows. The specimen shall be connected to the measurement apparatus shown in the block diagram of figure 10. The characteristic impedances of the specimen, the signal generator, the frequency counter, and the load impedance (Z_0) shall be identical. All interconnections shall be as short and free of electrical mismatch as possible.

The signal generator shall be set to a frequency that is five times the specified frequency, and varied until a Lissajous pattern on the screen of the oscilloscope forms a straight line. The positions of the signal generator and Z_0 shall then be reversed, and the oscilloscope screen observed. If a straight line is not now present, adjust the interconnections until a straight line is formed for both the normal and reversed positions of the signal generator and Z_0 .

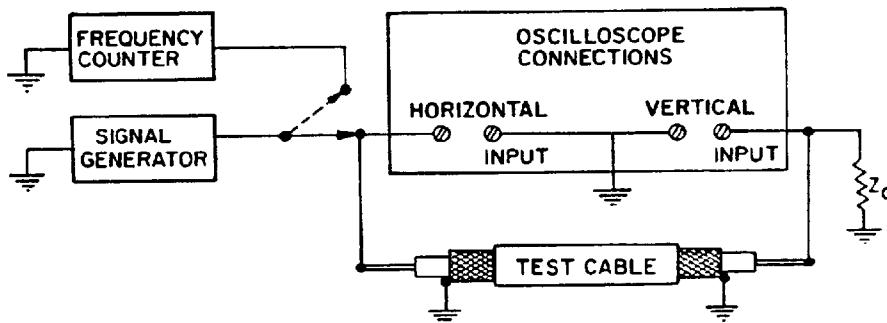


FIGURE 10. Block diagram of apparatus for measuring time delay.

Go back to the original position, by repositioning the apparatus as originally shown in the block diagram. Reset the frequency of the signal generator to the specified frequency and vary it until the Lissajous pattern displayed on the screen of the oscilloscope forms a straight line. The thickness of this line shall not exceed 0.01 inch to establish good resolution. A frequency counter shall then be temporarily inserted, as shown in the block diagram, to determine the exact frequency of the signal generator. This frequency shall then be recorded as the first resonance frequency (f_1). The frequency counter shall be removed, and the frequency of the signal generator shall be increased until the Lissajous pattern forms yet another line on the oscilloscope screen with the same direction as the first line. Again, the thickness of the line shall not exceed 0.01 inch. The frequency counter shall again be temporarily inserted to determine the second resonance frequency (f_2). This procedure shall be repeated until five successive frequencies have been determined. The time delay per foot of the cable shall then be computed as shown in the formula below. Beginning with the specified frequency, successive frequencies shall be determined, using this method.

$$TD = \left\{ \frac{1}{f_1} + \frac{2}{f_2} + \frac{3}{f_3} + \frac{4}{f_4} + \frac{5}{f_5} \right\} \frac{1}{5L}$$

Where: TD = Time delay, in microseconds per foot.

$f_1, 2, 3, 4, 5$ = Recorded frequencies, in MHz.

L = Specimen length, in feet.

The time delay shall be calculated for at least two sets of five successive recorded frequencies for each specimen. The average of these values computed shall be within the specified requirement (see 3.1). The specimen shall be reversed and the test repeated.

4.8.16 Aging stability (see 3.7.15).

4.8.16.1 Specimen. Four specimens shall be cut from the sample unit. For cables whose nominal jacket diameter is less than 0.5 inch, the specimen length shall be 125 ± 1 times the cable diameter. For cables whose nominal jacket diameter is 0.5 inch or larger, the specimen length shall be 95 ± 1 times the cable diameter. For armored cables, the armor shall be removed before the specimen is subjected to the aging stability test.

4.8.16.2 Procedure. The specimen shall be suspended in a heat chamber without touching one another or the walls of the chamber and conditioned for 7 days at the applicable test temperature in table XI. Test temperatures for cable jacket types not listed in table XI shall be as specified (see 3.1). Heated air shall be circulated so as to maintain a uniform test temperature. After the conditioning period, the specimens shall be removed from the heat chamber and conditioned at room ambient temperature for 4 hours minimum.

- Examine the specimen for cracks, flaws or other damage in the jacket material. For marked cables, examine the marking for legibility.
- Following the test, the specimen shall be subjected to the cold bend test (see 4.8.19).

TABLE XI. Jacket test temperature.

Jacket types	°C temperature
I, IIa, IV, and VIII	+98 ±2
IIIa	+90 ±2
V and VII	+250 ±5
VI	+200 ±5

4.8.17 Stress-crack resistance (see 3.7.16).

4.8.17.1 Specimen. Four specimens, approximately 3 feet long, shall be cut from the sample unit. For armored cables, the armor shall be removed before the specimen is subjected to the stress-crack resistance test.

4.8.17.2 Procedures. Clamp one end of each specimen to a mandrel whose diameter is three times the nominal jacket diameter of the cable unless otherwise specified (see 3.1). Wrap each specimen for 10 turns around the mandrel and clamp the specimen to the mandrel at this point. The specimens shall be suspended in a heat chamber without touching one another or the walls of the chamber and conditioned for 96 hours minimum at $+230^{\circ}\text{C} \pm 5^{\circ}\text{C}$. Heated air shall be circulated so as to maintain a uniform test temperature. After the conditioning period, the specimen shall be removed from the heat chamber and conditioned at room temperature for 4 hours minimum.

- a. Examine the specimen for cracks, flaws or other damage in the jacket material. For marked cables, examine the marking for legibility.
- b. Unwind the specimen from the mandrel and examine for cracks, flaws, or other damage in the jacket material. For marked cables, examine the marking for legibility.
- c. After the stress-crack resistance test, the specimen shall be subjected to the cold bend test (see 4.8.19).

4.8.18 Outer conductor integrity (see 3.7.17). Four specimens, approximately 2 feet long, shall be cut from the sample unit. The specimens shall be suspended in a heat chamber without touching one another or the walls of the chamber and conditioned for 1 hour 30 minutes minimum at the specified temperature (see 3.1). Heated air shall be circulated so as to maintain a uniform test temperature. After the conditioning period, the specimens shall be removed from the heat chamber and conditioned at room ambient temperature for 4 hours minimum. Examine the specimens for cracks, flaws, or other damage in the outer conductor material.

4.8.19 Cold bend (see 3.7.18). Three specimens shall be cut from the sample unit. The specimen lengths shall be the same as for the aging stability, stress-crack resistance and other outer conductor integrity tests, as applicable (see 4.8.16, 4.8.17, and 4.8.18). The distance between the cable turns wrapped on the mandrel shall not be more than the diameter of the cable; the cable shall make intimate contact with the mandrel.

4.8.19.1 Flexible cables.

- a. For armored cables, the armor shall be removed before the specimen is subjected to the cold bend test. One end of each specimen shall be clamped on a mandrel whose diameter is 10 times the normal outside diameter of the specimen in its present test condition. Wrap the specimen around the mandrel for one full turn and hold in place with a mechanical device. The specimens shall be placed in a cold chamber and conditioned for 20 hours minimum at the applicable test temperature. During the conditioning period, the unwrapped portion of the specimen shall be kept reasonably straight. The following details shall apply:
 - (1) For cables with type F dielectric cores, cables with type IIIa jackets, and cables whose nominal jacket diameter is .250 inch or smaller, the test temperature shall be $-55^{\circ}\text{C} \pm 2^{\circ}\text{C}$.
 - (2) For those other cables whose nominal jacket diameter is larger than .250 inch, the test temperature shall be $-40^{\circ}\text{C} \pm 2^{\circ}\text{C}$. For those cables that have been previously subjected to the aging stability test and stress-crack resistance tests, the test temperature shall be $-35^{\circ}\text{C} \pm 2^{\circ}\text{C}$.

- b. After the conditioning period and while the specimens are still at the test temperature, the specimens shall be wrapped around the mandrel for three full, close turns for cables whose nominal outside diameter is less than .500 inch, or two full close turns for cables whose nominal outside diameter is .500 inch or larger. The mandrel shall be turned at a uniform rate of 15 ± 3 revolutions per minute during this operation.
- c. After the turning operation, the specimen shall be removed from the cold chamber and conditioned at room ambient temperature for 1 hour maximum.

Unwind the specimen from the mandrel and, except at the clamping points, examine for cracks, flaws, or other damage in the outer surface material.

4.8.20 Dimensional stability (see 3.7.19).

4.8.20.1 Flexible cables. A 5-foot minimum specimen shall be cut from the sample unit. The ends of the specimen shall be cut squarely and carefully deburred. Place the specimen in a heat chamber, coiled or straight, and condition for 6 hours minimum at the applicable test temperature (see table XII). Heated air shall be circulated to maintain a uniform test temperature. After the conditioning period, remove the specimen from the heat chamber and condition at room ambient temperature for 4 hours minimum. Measure both ends of the specimen for protrusion or contraction of the inner conductor.

TABLE XII. Material and test temperature.

Material types	°C temperature <u>1/</u>
Type A dielectric	+85 ± 2
Type F dielectric (except with type IX jacket)	+250 ± 5
Type F dielectric with type IX jacket	+200 ± 5

1/ Test temperature for cable types not listed shall be as specified (see 3.1).

4.8.20.2 Semirigid cables.

- a. Specimen. An appropriate 4-foot length shall be cut from the sample unit and used to prepare six specimens. Each specimen shall have a length of $6.00 \pm .50$, $-.00$ inches with squared and carefully deburred ends. Each specimen shall be placed inside a brass test fixture as shown on figure 11.
- b. Procedure. After insertion of the specimen, the fixture ends shall be closed with caps; the caps shall be tightened with a torque of 8 inch-pounds ± 1 . Place the fixtures containing the captured specimens in a heat chamber and condition for at least 1 hour at the specified temperature (see 3.1). Heated air shall be circulated so as to maintain the test temperature within ± 5 degrees Celsius. After the conditioning period, the fixtures containing the specimens shall be maintained at room ambient temperature for at least 1 hour. Do not remove specimens from the test fixtures until immediately before measuring, and then remove one at a time. Measure the protrusion or contraction of the insulation with respect to the outer conductor on both specimen ends. Three measurements shall be made at each end, one in each of three different axial specimen orientations spaced approximately 120° apart, so that a total of six measurements are obtained for each specimen.

4.8.21 Contamination (see 3.7.20).

4.8.21.1 Specimen. The specimen length shall be 4 feet minimum for cables whose nominal outside diameter is more than 0.2 inch, 3 feet minimum for cables whose diameter is from 0.12 to 0.2 inch, and 2 feet minimum for cables whose diameter is less than 0.12 inch.

4.8.21.2 Equipment. Equipment for the contamination test shall be a Q-meter with an appropriate coil capable of giving an indicated Q-reading of 150 minimum. The resonating test frequency for all measurements shall be 1.2 MHz $\pm$ 50 kHz. Resonate the Q-meter to determine its Q-reading (Q_1).


4.8.21.3 Procedure. One end of the specimen shall be cut square. The other end shall be prepared to provide the shortest possible connection to the "high" terminal of the Q-meter. The shield shall be connected to the "ground" terminal. After attaching the specimen, resonate the Q-meter and take the new Q-reading (Q_2). This initial change in Q-readings (ΔQ_i) between the readings with and without the specimen attached shall be computed as $\Delta Q_i = Q_1 - Q_2$. If the initial change in Q (ΔQ_i) is less than three when using the specified length, the length may be increased so as to obtain a ΔQ_i of at least three. The specimen shall then be placed in a heat chamber and conditioned at $+98^\circ\text{C} \pm 2^\circ\text{C}$ for 7 days minimum. Heated air shall be circulated so as to maintain a uniform test temperature. After the conditioning period, the specimen shall be removed from the heat chamber and conditioned at room ambient temperature for 1 hour minimum. Again, with the specimen unattached, take a new Q-reading (Q_3). Attach the specimen as before and take another Q-reading (Q_4). This final change in Q-readings (ΔQ_f) between the readings with and without the specimen attached shall be computed as $\Delta Q_f = Q_3 - Q_4$. The change in ΔQ ($\Delta Q_f - \Delta Q_i$) shall not exceed the specified value (see 3.7.20).

4.8.22 Bendability (see 3.7.21). Two specimens, each approximately 1 foot long, shall be cut from the sample unit. The middle section of the specimen shall be formed for two complete turns around a mandrel of specified diameter (see 3.1) (Although no special tools are needed to guide the cable as it coils around the mandrel, a mechanism may be provided so as to avoid any damage to the outer conductor.) Remove the coiled specimen from the mandrel and examine the outer surface for cracks, splits, fracturing, and wrinkling.

4.8.23 Flammability (see 3.7.22).


4.8.23.1 Apparatus. The test shall be performed within a test chamber approximately 1 foot square by 2 feet in height, open at top and front to provide adequate ventilation for combustion but to prevent drafts. The specimen holder shall be designed so that the lower end of a 24-inch cable specimen is held by a clamp, while the upper end of the specimen passes over a pulley and can be suitably weighted to hold the specimen taut at an angle of 60 degrees with the horizontal, and in a plane parallel to and approximately 6 inches from the back of the chamber.

The separation between clamp and pulley shall be such that a minimum of 20 inches of the specimen is freely suspended. The test flame shall originate from a Bunsen type gas burner with a one-fourth inch inlet, a needle valve in the base for gas adjustment, three-eighth inch bore nominal, and an approximate 4-inch barrel length above the air inlets. The burner shall be adjusted to furnish a 3-inch conical flame with an approximate 1-inch long inner core and a flame temperature not less than 954°C (1749°F) at its hottest point, as measured with an accurate 1 percent full scale thermocouple pyrometer. A sheet of facial tissue conforming to UU-T-450 shall be suspended taut and horizontal 9-1/2 inches below the point of application of the flame to the cable specimen and at least one-half inch from the chamber floor, so that any material dripping from the cable specimen shall fall upon the tissue.

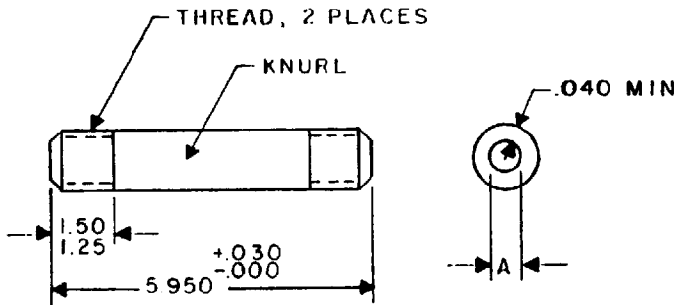

A DIMENSION = CABLE OD,
 $\pm .010$ MINIMUM, $.020$ MAXIMUM

FIXTURE BODY

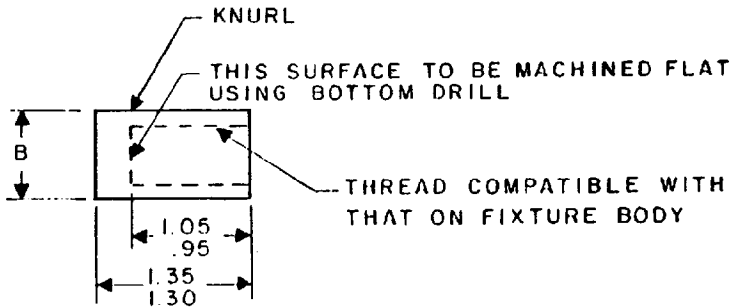

CAP (2 EACH)

INCHES	MM
.010	.25
.020	.51
.030	.76
.040	1.02
.95	24.1
1.05	26.7
1.25	31.8
1.30	33.0
1.35	34.3
1.50	38.1
5.950	151.13

"B" dimension not critical, but to provide for internal threading in accordance with standard shop practices.

NOTES:

1. Dimensions are in inches.
2. Metric equivalents are given for general information only.

FIGURE 11. Typical dimension stability test fixture.

4.8.23.2 Procedure. A 24-inch specimen of cable shall be marked at a distance of 8 inches from its lower end to indicate the point for flame application and placed in the specified 60-degree position in the test chamber. The lower end of the specimen shall be clamped in position in the specimen holder and the upper end shall be passed over the pulley of the holder and held taut. With the burner held perpendicular to the specimen and at an angle of 30 degrees from the vertical plane of the specimen, the hottest portion of the flame shall be applied to the lower side of the cable at the test mark. The test flame shall be applied for 30 seconds for all sizes of cable and then withdrawn immediately at the end of that period. The distance of flame travel upward along the specimen from the test mark and the time of burning after removal of the test flame shall be recorded; also the presence or absence of flame in the facial tissue due to incendiary drip from the specimen shall be recorded. Charred holes or spots in the tissue shall be ignored in the absence of actual flame. Breaking of the cable specimens in sizes 24 and smaller shall not be considered as failure provided the requirements for flame limits, duration of flame, and absence of incendiary dripping are met.

4.8.24 Weight (see 3.9). A section of cable shall be weighed on a scale that has a 0.1 percent accuracy.

4.8.25 Flame propagation (see 3.7.23). This test determines the relative ability of grouped cable to resist the propagation of fire along its length.

4.8.25.1 Specimen. Each specimen shall consist of a piece of completed cable which shall have a length of not less than 8 feet. The total number of specimens required shall be as specified in the vertical tray flame test of IEEE-STD-383.

4.8.25.2 Special apparatus. The apparatus shall include all equipment specified in the vertical tray flame test of IEEE-STD-383.

4.8.25.3 Procedure. The specimens shall be tested as specified in the vertical tray flame test of IEEE-STD-383.

4.8.25.4 Observation. Specimen failure shall be construed when any portion of any specimen burns to the top of the tray, either during or after operation of the ribbon burner. The following information (which does not constitute failure criteria) shall additionally be reported to help expand a performance data base: Flame temperature, period of time between burner shutoff and cessation of flame on the specimen, overall distance of specimen jacket damage above the burner, overall distance of specimen conductor damage above the burner, and a brief description of any dripping or flaming material which falls from the specimen to the floor during the test.

4.8.26 Acid gas generation (see 3.7.24). The method given below is to determine the total emission of any strong soluble acids (pH less than 3). The required apparatus is shown on figure 12. A weighed sample of the jacket, and insulation materials (for component wire, use insulation removed from a 22 AWG wire), normally 1/4 to 1/2 gram, shall be placed in a silica boat which is put into the center of a silica tube, length 50/60 centimeters and internal diameter 20/22 millimeters. The materials shall be tested individually. The silica tube shall be placed in the tube furnace. An air supply, derived from a blower or compressed air cylinder, at the rate of 1 liter per minute plus or minus 5 percent shall be passed through the silica tube and then through four absorber flasks each containing 30 milliliters of deionized water. The furnace heating shall be commenced and the temperature of the tube and sample shall be raised to $800 \pm 10^{\circ}\text{C}$ over a period of approximately 40 minutes and then held at temperature for a further 20 minutes. During the heating period, any acid gases produced will be carried over into the absorber flasks. On completion of the heating cycle, the acid content of the fluids in the absorber flasks shall be titrated against 0.1 N sodium hydroxide solution using congo red as an indicator. The total titre indicates the total soluble acids. 1.0 mL of 0.1 N sodium hydroxide solution is equivalent to 3.65 mg of acid expressed as 'acid equivalent relative to hydrochloric acid'.

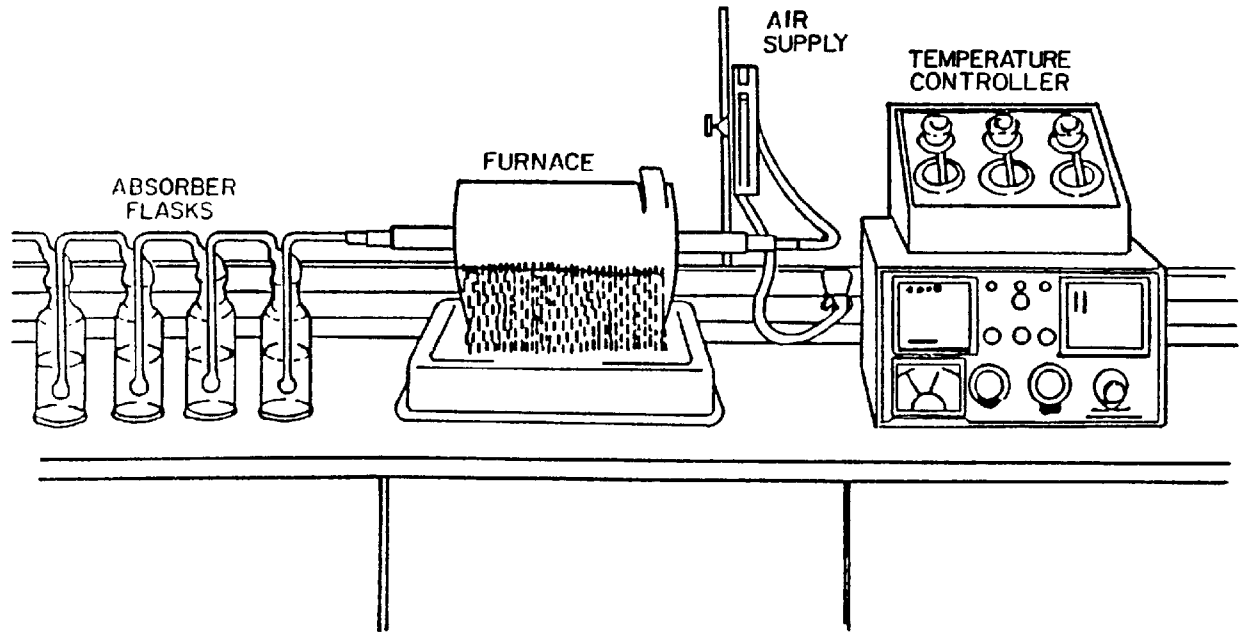


FIGURE 12. Acid gas test apparatus.

4.8.27 Halogen content (see 3.7.25). The halogen content of the cable jacket or fillers shall be determined by X-ray fluorescence or analytically following an examination and analyses of the chemical composition of all ingredients used.

4.8.28 Immersion tests (see 3.7.26). Specimens of the cable jacket material shall be immersed in the fluids shown in table XIII for 24 hours at the temperatures specified. The specimens shall then be removed, blotted to remove excess fluid, the suspended in air at room temperature for not less than 3 hours 30 minutes nor more than 4 hours 30 minutes. Each specimen shall be tested as specified in 4.8.37.

TABLE XIII. Immersion test temperatures.

Fluid	Test Temperature
Fuel oil, MIL-F-16884	98°C to 100°C
Turbine fuel, JP-4, MIL-T-5624	48°C to 50°C
Turbine fuel, JP-5, MIL-T-5624	48°C to 50°C
Cleaner, isopropyl alcohol, TT-I-735	20°C to 25°C
Hydraulic fluid, MIL-H-5606	48°C to 50°C
Hydraulic fluid, MIL-H-17672	48°C to 50°C
Lubricating oil, MIL-L-23699	98°C to 100°C
Lubricating oil, MIL-L-24467	98°C to 100°C
Coolant, Monsanto Coolanol 25 or equivalent	20°C to 25°C

4.8.29 Smoke index (see 3.7.27). The smoke index shall be measured as specified in NES 711 except the specimens for test shall be as follows:

- a. Jacket: Each specimen shall consist of a sufficient number of 75 mm long strips cut from the cable jacket to completely cover the face area of the sample holder. To prevent excessive buckling and distortion of the specimen during test, a wire mesh, manufactured from 1.0 mm diameter stainless steel wire with a spacing of 12.5 mm and a square mesh configuration, shall be placed inside and across the face of the sample holder. The specimen shall be fabricated by placing the specimen holder (with wire mesh) test face down onto a flat surface and positioning each 75 mm length in the holder in a parallel arrangement so that when the holder is in the test position the strips will be vertical. An insulating block 10 mm thick completely wrapped in aluminum foil shall be placed on top of the strips followed by a tension spring and locking pin.
- b. Insulation: The test specimen shall be a 1-meter length of 22 AWG finished wire.
- c. Fillers (when applicable): The test specimen shall be 3 by 3 inches of 0.070 inch thick block of the same material used in the cable.

4.8.30 Toxicity index (see 3.7.28). The toxicity index shall be determined as specified in NES 713. For insulation materials, the toxicity index shall be calculated on the mass of insulation on 1-meter length of finished wire size 22 AWG with a 0.5 mm wall thickness of insulation. For jacket and filler materials, the toxicity index shall be calculated on 100 grams of material. (the toxicity index is derived from the chemical analysis of the products of combustion of the materials.)

4.8.31 Durometer hardness (see 3.7.29). This test shall be to determine whether or not the jacketing material exhibits sufficient hardness for use in cable construction.

4.8.31.1 Specimen. The specimen shall consist of a block of material, of the dimensions specified in ASTM D-2240, which shall have been cured in effectively the same manner as when used in cable manufacture.

4.8.31.2 Special apparatus. Apparatus shall include a type A or type D durometer, as specified (see 3.1), which shall be in accordance with ASTM D-2240.

4.8.31.3 Procedure. The specimen shall be tested in accordance with ASTM D-2240.

4.8.32 Weathering. Jacket material shall be tested in accordance with ASTM D-2565. The following conditions shall apply:

Xenon arc lamp

6500 Watt

Borosilicate glass filters

Irradiance: 1.75 w/m^2 .nm at 500 nm

Exposure: Arc lamp on: 18 hours

Black panel temperature $50 \pm 2^\circ\text{C}$

Relative humidity 50 ± 2 percent

(for 18 minutes every 2 hours, water is sprayed onto specimen)

Arc lamp off: 6 hours

Temperature $35 \pm 2^\circ\text{C}$

Relative humidity 90-95 percent

Total exposure time: 1000 hours.

4.8.33 Abrasion resistance (see 3.7.31). Abrasion resistance of cable jacket material shall be determined as specified in 4.8.33.1 through 4.8.33.3.

4.8.33.1 Specimen. Cable jacket: The cable jacket test specimen shall be prepared by extruding material onto a 16 AWG (19/29) conductor. The material shall be manufactured using process conditions as close as possible to those used to produce the overall cable jacket and shall have an overall diameter of 0.119 plus 0.001, minus 0.000 inch.

4.8.33.2 Special apparatus. Apparatus shall include the following:

- a. Abrading machine: A cylinder, which incorporates two abrading elements on its surface, which is motor driven to rotate about a horizontal axis at 17 plus 3, minus 2 revolutions per minute (r/min) and over which the specimen is draped, as shown on figures 13 and 14, and as described below:

- (1) Each abrading element shall consist of 5/16 inch square, high-speed tool bit (Cleveland Twist Drill Company number 855 or its equivalent) which has been ground on two adjacent, longitudinal sides to produce a single, sharp 90 degree longitudinal edge, free of visible nicks. A medium grade grinding wheel (Norton Company number 39C6018VK or its equivalent) shall be used for this grinding. Abrading elements shall be reground as required; in no case shall an abrading element be used in excess of 5 hours without regrinding. Whenever the perpendicular distance between either pair of opposite longitudinal sides of an abrading element becomes less than 0.3085 inch (as by repeated regrinding) then that abrading element shall be discarded and replaced.
- (2) The cylinder shall be $8 \pm 1/8$ inches in diameter and shall be rigidly fabricated from metal.

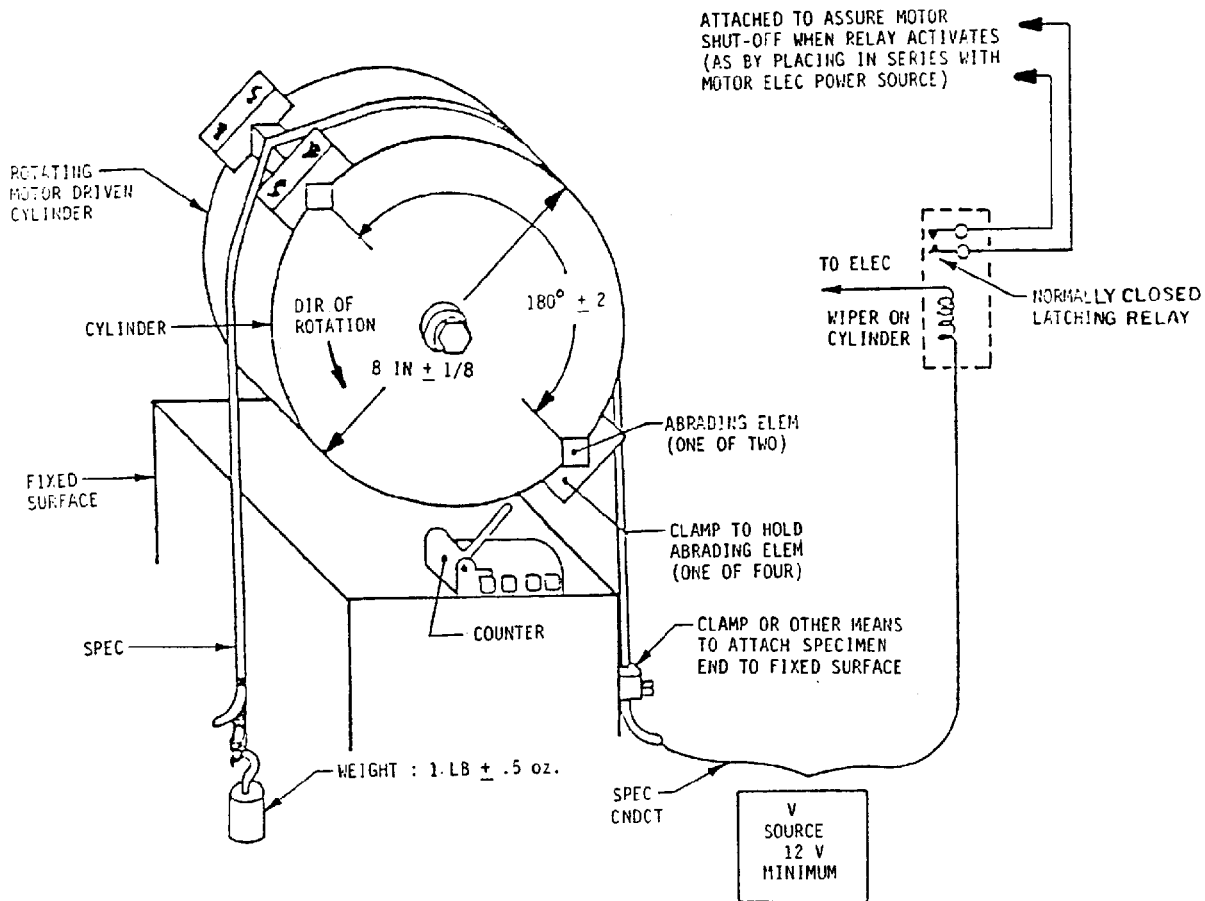


FIGURE 13. Diagram of abrading machine for the abrasion resistance test.

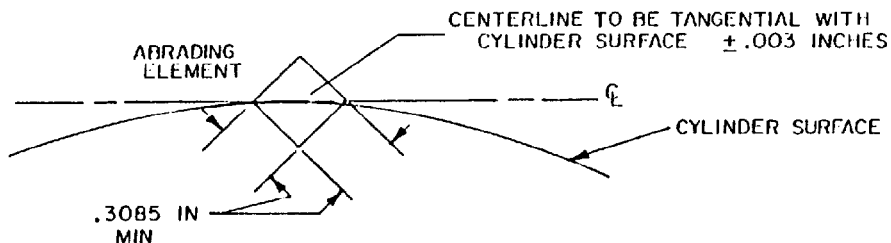


FIGURE 14. Detail diagram of abrading element fit on cylinder surface.

(3) Each of the two abrading elements shall be maintained in electrical contact with the metal cylinder by securing each in a notch cut into the cylinder surface, parallel to the cylinder axis; the two notches required shall be spaced 180 ± 2 degrees apart around the circumference of the cylinder. These notches shall be cut such that the sharpened 90 degree longitudinal edge of each element shall be facing outward from the cylinder surface, and such that the midpoint of a straight line drawn between the two longitudinal edges adjacent to the sharpened edge is tangential plus or minus 0.003 inch to the cylinder surface.

(4) An automatic counter shall be provided to totalize the number of times that the specimen is scraped by abrading elements during the test.

(5) A 1 pound ± 0.5 ounce weight shall be provided for applying tension to the specimen.

- b. Short circuit monitor: A voltage source of not less than 12 V (either direct current (dc) or root mean square (rms) alternating current (ac) which can be applied between the specimen conductor and both abrading elements of the abrading machine as shown on figure 13. (The connection to the abrasion elements may be provided by a wiping contact on the cylinder.) A means (such as an electrical relay) shall be provided whereby an electrical connection between either abrading element and the specimen conductor shall automatically stop rotation of the cylinder on the abrading machine (as by removing motor power).

4.8.33.3 Procedure. The specimen shall be wiped with a clean, dry cloth to remove any lubricant or dirt. The specimen shall then be tested (either simultaneously or one at a time) as follows. The specimen shall be hung circumferentially over the cylinder of the abrading machine, such that the specimen shall form an arc of not less than 170 degrees around the cylinder for the remainder of the test. One end of the specimen shall then be secured to a fixed surface. The abrading machine weight shall be attached to the opposite specimen end, such that both the specimen end and the weight shall be freely suspended. The automatic counter shall be set initially to zero, and the short circuit monitor shall be applied between both abrading elements on the abrading machine and the conductor of the specimen. The cylinder motor shall then be turned on, allowing the cylinder to rotate beneath the specimen, from secured end to the weighted end.

4.8.34 Tear strength (see 3.7.32). This test shall determine the ability of elastomeric jacketing material to withstand the propagation of a cut passing through a portion of its length.

4.8.34.1 Specimen. The specimen shall consist of a piece of jacketing material cut to the dimensions specified in ASTM D-470. The specimen shall be removed from a completed cable.

4.8.34.2 Special apparatus. Apparatus shall include the following:

- a. A micrometer with flat, parallel measurement surfaces on both spindle and anvil, which shall be for the specimen measurements as specified in 4.8.34 and which shall exhibit a measurement error of not more than plus or minus 0.001 inch.

- b. A motor driven tensile machine which shall be for applying increasing tension to the specimen, and which shall automatically indicate within plus or minus 1 percent the maximum tension experienced by the specimen prior to tearing. This tensile machine shall incorporate two parallel and opposing jaws, between which the specimen can be secured, as specified in 4.8.34.3. The two jaws shall increase their separation at the uniform rate of 20 ± 2 inches per minute by means of the tensile machine motor.

4.8.34.3 Procedure. The specimen shall be tested in accordance with ASTM D-470.

4.8.35 Heat distortion (see 3.7.33). This test shall determine the ability of the jacket material to resist physical deformation when subjected to an elevated temperature.

4.8.35.1 Specimen. The specimen shall be removed from completed cable in accordance with 4.8.35.1.2.

4.8.35.1.2 Cable jacket. The specimen shall consist of a piece of jacketing that has been removed from a finished cable and cut to form a rectangular strip. This strip shall be not less than $7/8$ inch long nor less than $9/16 \pm 1/16$ inch wide, and shall be ground and buffed to a thickness of 0.050 ± 0.010 inch with a grinding apparatus (see 4.8.35.2b). The thickness of the specimen shall be made as uniform as practicable.

4.8.35.2 Special apparatus. Apparatus shall include the following:

- a. A self-standing thickness gauge, for supporting the requirements as specified in 4.8.35.3, which shall exhibit a measurement error of not more than plus or minus 0.001 inch. This gauge shall incorporate a flat horizontal platen upon which an entire specimen shall be laid flat during measurement, and shall incorporate a foot which rests upon the top of the specimen during measurement. This foot shall be attached to a plunger which moves freely in the vertical direction, and which is attached to a dial or other indicating device from which the specimen thickness may be read. The foot shall present a horizontal disk of $3/8$ plus 0, minus $1/64$ inch diameter to the specimen, shall bear down upon the specimen with a force of 85 plus 0, minus 4 grams and shall be loaded with weights (see 4.8.35.3) to present additional force to the specimen.
- b. A motor driven grinding wheel and a motor driven buffing wheel, or their equal, for the specimen preparation as specified in 4.8.35.1.2. Guides shall be provided to assure that the specimen is pulled tangentially to the surface of each wheel during grinding and buffing.
- c. An oven, for accommodating the gauge with specimen inserted and for supporting the requirements as specified in 4.8.35.3. The oven air temperature shall be measured in the immediate vicinity of the specimen.

4.8.35.3 Procedure. The initial jacket material thickness of the specimen (T in formula below) shall be determined (see a below) and the oven shall be preheated to 121 ± 1 C. This oven temperature shall be maintained for the remainder of the test. The gauge foot shall then be loaded with weights (see b. below) and the gauge placed within the oven. Not less than 1 hour later, the specimen shall be placed in the oven. Not less than 1 hour after placing the specimen in the oven, the specimen shall be placed beneath the gauge foot such that the gauge indicates the specimen thickness. Not less than 1 hour after placing the specimen beneath the gauge foot, the final specimen thickness shall be read from the gauge and the final insulation thickness (t in formula below) determined (see c. below). In an identical manner, the remaining specimens shall also be tested. The percentage heat distortion of the jacket material shall then be calculated by using the following formula:

Percentage heat distortion = Median value of $100(T-t)/T$ for all tested specimens.

Where: T = Initial jacket material thickness of the specimen, in thousandths of an inch (see a. below).
 t = Final jacket material thickness of the specimen, in thousandths of an inch (see c. below).

The following additional details apply:

- a. The initial jacket material thickness (T) shall be the initial specimen thickness, as measured with the gauge, prior to loading the gauge with weights and prior to inserting either the gauge or the specimen into the oven.
- b. The gauge foot shall be loaded with 2000 $\pm$ 100 grams.
- c. The final jacket material thickness (t) shall be the final specimen thickness, measured as specified.

4.8.36 Physical tests on aged jacket (see 3.7.34). This test shall determine whether or not various jacketing materials have been properly processed, by means of tensile measurements. This test makes provision for making tensile measurements both before and after these materials have been artificially aged.

4.8.36.1 Specimens. Each specimen shall consist of a single piece of jacketing, which shall have sufficient length for use in the tests as specified in 4.8.37, as specified (see 3.1). Specimens shall be removed from completed cable.

4.8.36.2 Special apparatus. Apparatus shall include the following:

- a. A forced-fresh-air circulating oven for supporting the requirements as specified in 4.8.36.3a. The oven air temperature shall be measured in the immediate vicinity of the specimens.
- b. A heated container, which shall be filled with lubricating oil in accordance with symbol number 2190 TEP of MIL-L-17331, and which shall be for the specimen immersion as specified in 4.8.36.3b. The oil shall be maintained at a temperature of 121 $\pm$ 1°C during specimen immersion.

4.8.36.3 Procedure. Specimens shall be maintained at ambient temperature for a period of not less than 30 minutes immediately prior to any accelerated aging or testing. Each of the specified accelerated aging procedures shall be performed as follows, using one specimen for each procedure. The same specimen shall not be used for more than one procedure. Each of the specified tests shall be performed as specified in 4.8.37.

- a. Air oven accelerated aging: Each specimen shall be freely suspended vertically, secured by one end, within the oven. The air temperature within the oven shall then be raised to the value specified in table XIV, and shall be maintained at this value for a continuous period of not less than that specified in table XIV. Each specimen shall then be removed from the oven and tested as specified in 4.8.37.
- b. Hot-oil immersion accelerated aging: Each specimen shall be submerged within the hot oil bath for a continuous period of not less than that specified in table XIV. Each specimen shall then be removed from the hot oil bath, blotted lightly to remove excessive oil and then suspended in air, to ambient room temperature, for 4 hours $\pm$ 30 minutes. Each specimen shall then be tested as specified in 4.8.37.

4.8.37 Tensile strength and elongation (see 3.7.35). Both aged and unaged specimens of the insulation and jacket material shall be tested in accordance with methods 3021 and 3031 of FED-STD-228. Unless otherwise specified on the applicable specification sheet, there shall be 1-inch bench marks, 1-inch jaw separation, and a rate of jaw travel of 10 inches per minute. The thickness of the specimen shall be measured using any suitable micrometer.

TABLE XIV. Details for accelerated aging procedures.

Specimen material	Procedure	Temperature (°C)	Minimum period (hours)
Jacketing specimen: Cross-linked polyolefin	Air oven Hot-oil immersion	136 ±2 121 ±1	168 18

5. PACKAGING

5.1 Packaging requirements. The requirements for packaging shall be in accordance with MIL-C-12000.

6. NOTES

(This section contains information of a general or explanatory nature that may be helpful, but is not mandatory.)

6.1 These cables are intended for use in radio frequency applications. Reference MIL-C-39012 for compatible connectors.

6.2 Acquisition requirements. Acquisition documents should specify the following:

- Title, number and date of this specification.
- Title, number and date of the applicable specification sheet.
- Complete cable part number (see 1.2.1).

6.3 International standardization agreements. Certain provisions of this specification are the subject of international standardization agreement, NATO NEPR No. 3. When amendment, revision, or cancellation of this specification is proposed which affects or violates the international agreement concerned, the preparing activity will take appropriate reconciliation action through international standardization offices, if required.

6.4 Qualification. With respect to products requiring qualification, awards will be made only for products which are at the time set for opening of bids, qualified for inclusion in applicable qualified products list (QPL) whether or not such products have actually been so listed by that date. The attention of the contractors is called to this requirement, and manufacturers are urged to arrange to have the products that they propose to offer to the Federal Government tested for qualification in order that they may be eligible to be awarded contracts or orders for the products covered by this specification. The activity responsible for the qualified products list is the U.S. Army Communications-Electronics Command, Fort Monmouth, New Jersey 07703; however, information pertaining to qualification of products may be obtained from the Defense Electronics Supply Center (DESC-E), Dayton, Ohio 45444.

6.5 Definitions.

6.5.1 Maximum continuous working voltage. The maximum continuous working voltage is that safe voltage that can be continuously applied to a coaxial cable. This voltage is limited by the onset of corona breakdown. The cable working rating is 75 percent of the corona extinction corona voltage rating.

6.5.2 Maximum operating frequency. Coaxial cables operate in the principal or transverse electromagnetic (TEM) mode. The TEM mode has both the electric and magnetic field lines normal to the direction of propagation. The possibility of propagation in the higher modes limits the usefulness of a coaxial cable to below the lowest higher-mode cut-off frequency. To determine a maximum operating frequency it is necessary to derate from the cut-off frequency to forestall the operation of the cable in a mode higher than the TEM mode. Other factors that contribute to a lower operating frequency are the elements of construction of the cable and the associated connectors. The recommended maximum operating frequency takes into account all of these factors, but the user should always check the capabilities of cable and connector assembly before operating at any high frequency.

6.5.3 Velocity of propagation (VP). The velocity of propagation (VP) is the velocity of an electric wave governed solely by the properties of the dielectric medium and the permeability of the conductor through which it is transmitted. In free space the electromagnetic energy will travel with a speed of 3×10^8 meters per second or a 100 percent VP. In a coaxial cable with a uniform dielectric and a conductor with a relative permeability of 1, the VP is always less than 100 percent. Hence, the VP of a coaxial cable is the ratio of the speed of electromagnetic energy flow compared to the speed of light.

$$\% VP = \frac{\text{Velocity of energy in a cable dielectric medium}}{\text{Velocity of energy in free space}} \times 100\%$$

The VP in a cable may be found by resonating a length of cable at 100 MHz or more, with one end short-circuited or open-circuited in accordance with the following formula:

$$\% VP = \frac{f_r \times \text{Cable length (feet)}}{2.46 \times N}$$

Where: N = Number of quarter wavelengths in the cable specimen.

f_r = Resonant frequency.

A simpler method of computing the % VP uses the effective dielectric constant of the dielectric medium.

$$\% VP = \frac{1}{\sqrt{e}} \times 100\%$$

6.5.4 Power rating (CW). The maximum power-handling capability, in watts, is the amount of power that a coaxial cable can safely transmit without overheating or developing a dielectric breakdown throughout the usable frequency range. The safe power-handling capabilities are shown on the associated curves. These curves have been derated with an assumption of a VSWR of 2, an ambient temperature range of +38°C to +71°C for PE dielectric, and +38°C to +149°C for PTFE dielectric, and also a maximum inner conductor temperature of +85°C for PE and +200°C for PTFE. The curves have also taken into account the effects of typical system installations (i.e., bends, clamps, thermally insulated sections, etc.).

6.5.5 Coaxial connectors. The applicable connector series is given on the specification sheet, although many other connectors are constructed particularly for these coaxial cables. Extreme care shall be taken in handling a coaxial cable for assembly to connectors so as not to work-harden, overheat, or damage the cable components.

6.5.6 Minimum recommended bend mandrel radius for normal use. The minimum recommended bend radius for a coaxial cable in normal usage is given on the specification sheet. The radius given is to the outer surface of the cable. This minimum bend radius is dependent upon the material of the outer conductor and its thickness. If possible and the attenuation requirements allow it, add a service length to the cable. Do not use tight bend radii unless the application warrants it. Extreme care should be taken in the forming to prevent wrinkling or cracking.

6.5.7 Operating temperature range. The operating temperature range is the limits between which a cable may be operated continuously without any loss in the basic properties of the cable. This includes the ambient temperature plus the increased temperature due to inner conductor operation. This temperature range is just a guideline, since the mechanical, environmental and electrical requirements of the application contribute to the allowable temperature range. In no case should the testing temperatures be considered as the operating temperature range. Testing is usually done under accelerated conditions so as to possibly degrade the materials.

6.5.8 Maximum operating temperature for semirigid cables. Heating semirigid cables and cable assemblies to exceed specified temperatures (see 3.1) will cause permanent increases in the outer conductor diameter. These, in turn, will increase the characteristic impedance, decrease conductor adherence capacitance and corona extinction voltage, and cause VSWR increases in cable assemblies. While effects of temporary heating during soldering processes can be minimized or eliminated, the effects of long-term heating of semirigid cables and cable assemblies must be taken into consideration by the designers.


6.6 Preconditioning semirigid cables.

- a. The electrical and mechanical performances specified for semirigid cables are achieved by a compression fit between the outer conductor and the dielectric core which, in turn, necessitates manufacturing processes that cause deformation of the core by compression and elongation. The resulting stress that is initially nonuniform tends to equalize by cold flow within a few weeks after the manufacturing, and will cause withdrawal of the core into the cable. If this occurs in cable that has become part of a cable assembly, the resultant development of an air-void at the cable-conductor interface causes VSWR increase. It is therefore advantageous to achieve core stress relief by preconditioning cable before it becomes a cable assembly.
- b. Preconditioning is not effective on long lengths of cable. Bending of cable, which is usually involved in the manufacture of cable, tends to introduce nonuniform core stresses; therefore, preconditioning is more effective when performed on cable assemblies that are complete except for the final end preparation and before attaching the connector. Since preconditioning will result in withdrawal of dielectric into the cable, preparation of the cable assembly should allow for a 1/4-inch length on each cable end beyond the design dimension. The outer conductor and the core should not be cut to the final dimensions until preconditioning has been completed.


- c. A recommended preconditioning procedure consists of three of the following temperature cycles:
- (1) Step 1. Heat the specimen to the maximum operating temperature specified (see 3.1) and maintain for 1 hour minimum.
 - (2) Step 2. Return specimen to room ambient temperature. Trim protruding core, if any, flush with the edge of the outer conductor.
 - (3) Step 3. Maintain specimen at room temperature for 1 hour minimum.
 - (4) Step 4. Cool specimen to -45°C and maintain for 1 hour minimum.
 - (5) Step 5. Return specimen to room temperature and maintain for 1 hour minimum.
- d. After the last temperature cycle, maintain the specimen at room temperature for 24 hours minimum before proceeding with further processing.
- e. Recommendations for dealing with special requirements should be obtained from cable manufacturers.

6.7 Suggested method for making cable ends corona-free is shown on figure 15.


Step 1: Suggested length of cable specimen is 36.00 inches (914.40 mm).

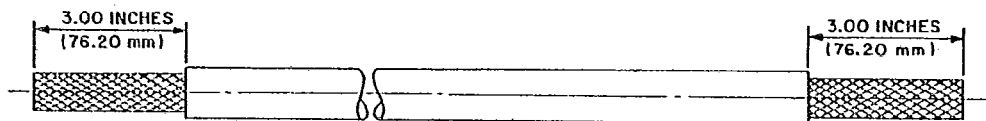

Step 2: Remove 3.00 inches (76.20 mm) of jacket material from each end.

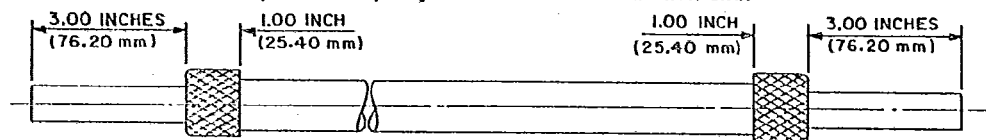

Step 3: Roll back the braid over the jacket and trim as shown. Be careful to avoid breaking any strands. Trim the braid edges neatly to 1.00 inch (25.40 mm) lengths.

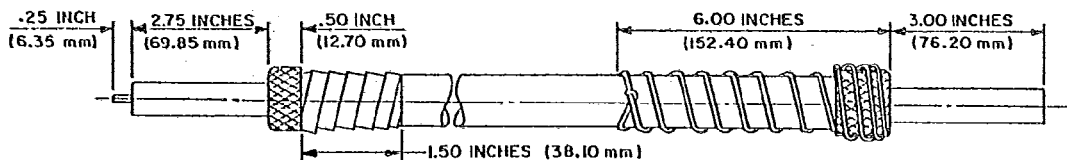

Step 4: Trim one end of the specimen to the dimensions shown and cover the braid edge and jacket with a plastic tape as shown. Wrap an AWG No. 20 copper grounding wire tightly over the braid.

FIGURE 15. Suggested method for making cable ends corona free.

6.8 Part or Identifying Number. The PIN shall consist of the following:

	<u>M17</u>	<u>/XXX-</u>	<u>XXXXX</u>
Basic specification _____			
Specification sheet (use minimum number of digits) _____			
RG number or new number (5 places in length) _____			

Example of existing RG number - M17/28-RG058

Example of new number - M17/155-00001

6.9 Key word listing.

Coaxial
Coax
Triaxial
Triax
Twinaxial
Twinax
RF Cable
Electrical
Microwave

NOTE: Asterisks are not used in this revision to identify changes with respect to the previous issue due to the extensiveness of the changes.

APPENDIX

PROCEDURE FOR GROUP QUALIFICATION INSPECTION

10. SCOPE

10.1 This appendix details the procedure for group qualification inspection of cables covered by this specification. The procedure for extending qualification of the required sample to other cables covered by this specification is also outlined herein.

20. APPLICABLE DOCUMENTS. This section is not applicable to this appendix.

30. EXTENT OF QUALIFICATION

30.1 Group qualification. The cable types listed in column 3 of table XV are eligible for group qualification. The groups are based on similar characteristics and requirements. At the discretion of the Government, qualification may be extended to cover any or all cable types in a group, based on compliance of one cable type in that group with the qualification inspection. The Government reserves the right to authorize performance of any or all qualification inspection on additional types in the group that are considered necessary to the extension of qualification within each group. Cable types not included in these groups are not eligible for group qualification. Group qualification will be granted final acceptance contingent upon receipt of successful retention of qualification data for individual cables within 2 years.

TABLE XV. Group qualification. 1/ 2/ 3/

Group	Submission and qualification of any of the following cable types	Qualifies the following cable types
I	M17/84-RG223	M17/167-00001
II	M17/60-RG142	M17/111-RG303, M17/158-00001, M17/170-00001
III	M17/67-RG177	M17/79-RG318, M17/78-RG217, M17/160-00001, M17/165-00001, M17/166-00001
IV	M17/137-00001	M17/139-00001
V	M17/65-RG165	M17/86-00001, M17/159-00001
VI	M17/152-00001	M17/113-RG316
VII	M17/131-RG403	M17/93-RG178, M17/169-00001
VIII	M17/28-RG058	M17/155-00001
IX	M17/52-RG119	M17/156-00001
X	M17/54-RG122	M17/157-00001

APPENDIX

TABLE XV. Group qualification - Continued.

Group	Submission and qualification of any of the following cable types	Qualifies the following cable types
XI	M17/72-RG211	M17/161-0001
XII	M17/73-RG212	M17/162-00001
XIII	M17/74-RG213	M17/74-RG215, M17/163-00001
XIV	M17/75-RG214	M17/164-00001
XV	M17/92-RG115	M17/168-00001
XVI	M17/112-RG304	M17/171-00001
XVII	M17/119-RG174	M17/173-00001
XVIII	M17/127-RG393	M17/174-00001
XIX	M17/128-RG400	M17/175-00001
XX	M17/93-RG178	M17/169-00001

- 1/ Swept cables automatically qualify their nonswept counterpart (i.e., M17/28-RG058 qualifies M17/155-00001).
- 2/ Qualification of an unarmored cable automatically qualifies its armored version, when requested by the manufacturer.
- 3/ Qualification of any semi-rigid cable in a series described by a single detail specification sheet automatically qualifies any other version in the same series, when requested by the manufacturer.

APPENDIX

CONCLUDING MATERIAL

Custodians:

Army - CR
Navy - EC
Air Force - 85

Preparing activity:

Army - CR

Agent:

DLA - ES

(Project 6145-1116)

Review activities:

Army - AR, MI
Navy - SH
Air Force - 11, 17, 99
DLA - ES, IS
NASA - NA

User activities:

Army - ME, AT
Navy - AS, OS, MC
Air Force - 19